

Xenium In Situ for Fresh Frozen Tissues – Fixation & Permeabilization

Introduction

Xenium In Situ for Fresh Frozen Tissues is designed to measure mRNA in fresh frozen tissue sections and requires a Xenium slide with intact tissue sections as input. This protocol outlines fixation and permeabilization of fresh frozen tissue for use with 10x Genomics Xenium In Situ Gene Expression protocols. Fixed and permeabilized tissue sections are inputs for the downstream Xenium In Situ Gene Expression - Probe Hybridization, Ligation & Amplification workflow.

Additional Guidance

Consult the Xenium In Situ for Fresh Frozen - Tissue Preparation Guide (Document CG000579) for complete information on sectioning fresh frozen tissue and placing sections on Xenium slides. After completing this Demonstrated Protocol (CG000581), proceed with the Xenium In Situ Gene Expression - Probe Hybridization, Ligation & Amplification User Guide (CG000582).





Contents


Xenium In Situ Gene Expression Reagent Kits	3
Xenium Decoding Consumables (1 run, 2 slides) PN-1000487	3
Xenium Instrument Accessory Kit Module A PN-1000530	3
Xenium Cassette Kit - (2 cassettes) PN-1000566	4
Recommended Thermal Cyclers	5
Workflow Overview	6
Specific Reagents & Consumables	7
Tips & Best Practices	9
Icons	9
Pipette Calibration	9
Xenium Slide	10
Slide Storage	11
Xenium Slide Handling	12
Xenium Cassette	13
Xenium Cassette Assembly	15
Xenium Cassette Removal	16
Reagent Addition to Wells	17
Reagent Removal from Wells	17
Xenium Cassette Lid Application & Removal	18
Slide Incubation Guidance	19
Tissue Detachment on Xenium Slides	20
Protocol Steps & Timing	21
1. Fixation & Permeabilization	22
1.0 Overview	22
Protocol Overview	23
Get Started - Fixation & Permeabilization	24
1.1 Preparation - Buffers	25
1.2 Slide Preparation	28
1.3 Fixation	29
1.4 Permeabilization	30
1.5 Cassette Assembly	31
Troubleshooting	32
Document Revision Summary	34

Xenium In Situ Gene Expression Reagent Kits

Refer to SDS for handling and disposal information

Xenium Decoding Consumables (1 run, 2 slides) PN-1000487

Xenium Decoding Consumables (1 run, 2 slides), PN-1000487 <i>Store at ambient temperature</i>	
	# PN
Xenium Cassette Kit (2 cassettes + 16 lids)	1 1000566
Extraction Tip	1 2000757
Pipette Tips	1 3000866
Xenium Buffer Cap	4 3000949
Xenium Objective Wetting Consumable	1 2000749
 Deionized Water (bottle)	1 3001198
 Xenium Sample Wash Buffer A (bottle)	1 3001199
 Xenium Sample Wash Buffer B (bottle)	1 3001200
 Xenium Probe Removal Buffer (bottle)	1 3001201



Only the Xenium Cassette Kit (2 cassettes + 16 lids) (PN-1000566) is needed for this workflow.

Xenium Instrument Accessory Kit Module A PN-1000530

Xenium Instrument Accessory Kit Module A PN-1000530 <i>Store at ambient temperature</i>		
	#	PN
Waste Bottle	1	3000955
Xenium Waste Tip Tray	1	3000957
Xenium Thermocycler Adaptor	1	3000954



Only the Xenium Thermocycler Adaptor (PN-3000954) is needed for this workflow.

Xenium Cassette Kit - (2 cassettes) PN-1000566

Xenium Cassette Kit (2 cassettes) PN-1000566 <i>Store at ambient temperature</i>		
	#	PN
Xenium Cassette lids (16 ct)	1	3001046
Xenium Cassettes (2 pack)	1	3000951



Purchase the Xenium Cassette Kit (2 cassettes) (PN-1000566) for additional cassettes as needed.

Recommended Thermal Cyclers

Supplier	Description	Part Number
Bio-Rad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module (discontinued)	1851197
Analytik Jena	Biometra TAdvanced 96 SG with 96-well block (silver, 0.2 mL) and gradient function	846-x-070-241 (where x=2 for 230 V; 4 for 115 V; 5 for 100 V, 50-60 Hz)
VWR	Gradient thermal cycler, XT ⁹⁶ Gradient, with 96-well gradient block and standard lid	76452-153
Marshall Scientific	MJ Research PTC-200 Thermal Cycler	05434-05

Workflow Overview

Tissue Preparation Guide

Section Fresh Frozen tissue onto slides
Demonstrated Protocol CG000579



Fixation & Permeabilization

Fix and permeabilize tissue
Demonstrated Protocol CG000581



Probe Hybridization, Ligation & Amplification

For FF & FFPE Samples on Xenium Slides
User Guide CG000582



Decoding & Imaging

Load Xenium Cassette onto Xenium Analyzer
User Guide CG000584



Optional:

H&E Staining

H&E Stain post-Xenium run
Demonstrated Protocol CG000613

Visit the [10x Genomics Support website](https://support.10xgenomics.com) for the most current documentation.

Specific Reagents & Consumables

Fresh Frozen Tissue Sections: Fixation & Permeabilization

The listed items have been tested by 10x Genomics and perform optimally with the assay.

Substituting materials may adversely affect system performance. For items with multiple options listed, choose option based on availability and preference. Refer to the manufacturer's website for regional part numbers.

For FF Tissue Sections: Fixation & Permeabilization				
	Item	Description	Vendor	Part Number
<input type="checkbox"/>	PBS	PBS - Phosphate Buffered Saline (10X) pH 7.4, RNase-free	Thermo Fisher Scientific	AM9624
<input type="checkbox"/>	Nuclease-free Water	Nuclease-free water (not DEPC-treated)	Thermo Fisher Scientific	AM9932/ AM9937
<input type="checkbox"/>	Formaldehyde	Formaldehyde (37% by Weight/Molecular Biology)	Thermo Fisher Scientific	BP531-500
	or	Formaldehyde Solution	Millipore Sigma	252549, F8775, or 47608
	Paraformaldehyde	Paraformaldehyde 16% Aqueous Solution, EM Grade	Electron Microscopy Sciences	15710
<input type="checkbox"/>	Ethanol	Ethyl Alcohol, 200 Proof, anhydrous	Millipore Sigma	E7023
		Ethanol absolute ≥99.5%, TechniSolv, pure (Europe Only)	VWR	83813.360DP
<input type="checkbox"/>	10% Tween-20	Tween 20 Surfact-Amps Detergent Solution (10% solution)	Thermo Fisher Scientific	28320
		(not 100% Tween diluted to 10%)		
		10% Tween-20	Bio-Rad	1662404
<input type="checkbox"/>	Methanol	Methanol, for HPLC	Millipore Sigma	34860
<input type="checkbox"/>	SDS	Sodium dodecyl sulfate solution (for molecular biology, 10% in H2O)	Millipore Sigma	71736
<input type="checkbox"/>	Forceps	Tweezers, 4" Wafer Handling	Excelta Corp	491P-SA-PI
<input type="checkbox"/>	Slide Mailers	Sim port Scientific LockMailer Tamper Evident Slide Mailer	Fisher Scientific	22-038-399
Additional Materials				
<input type="checkbox"/>	Dry Ice			
<input type="checkbox"/>	Thermal Cycler (see Recommended Thermal Cyclers)			
<input type="checkbox"/>	Slide drying rack			
<input type="checkbox"/>	Fume Hood			

For FF Tissue Sections: Fixation & Permeabilization

- Vortex
 - Ice bucket
-

This list may not include some standard laboratory equipment.

Tips & Best Practices

Icons



Tips & Best Practices section includes additional guidance



Signifies critical step requiring accurate execution



Troubleshooting section includes additional guidance

General Reagent Handling


- Fully thaw reagents at indicated temperatures. Thoroughly mix reagents before use.
- When pipette mixing reagents, unless otherwise specified, set pipette to 75% of total volume.
- Promptly move reagents back to the recommended storage.

Pipette Calibration

- Follow manufacturer's calibration and maintenance schedules.

Xenium Slide

- Xenium slides include an imageable area outlined by a white line measuring 12 mm x 24 mm, with an available sample positioning area measuring 235 mm² (10.45 mm x 22.45 mm). The available sample positioning area will be referred to as the Sample Area for the remainder of this document.
- The Sample Area is surrounded by fiducials. Tissue sections are placed within the Sample Area without obstructing the fiducials. The imageable area includes the area within the fiducial frame + Sample Area.
- The Sample Area can accommodate as many tissue sections as can fit within the space. Ensure tissue sections (including OCT) DO NOT overlap.
- An etched label denoting the Slide ID, Part, and Version numbers is located at the bottom of the slide. Tissue sections should be placed on labeled-side of slide.

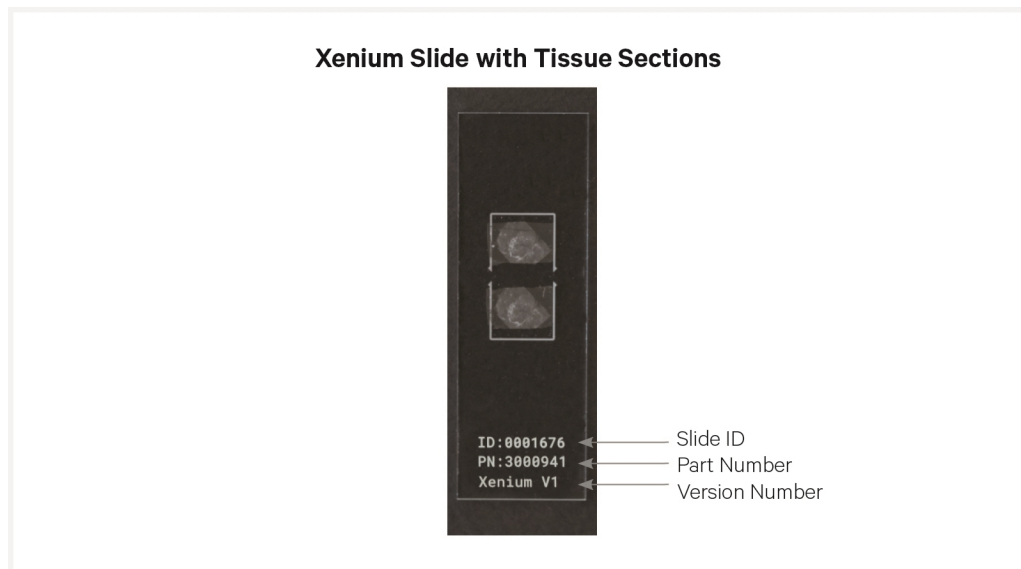

Slide Storage

- Always store unused slides at -20°C in their original packaging and keep sealed. Once opened, slides should remain at room temperature in a desiccator and be used within one week.
- After tissue placement, store slides in a sealed container. If using an unsealed slide mailer, store in a secondary sealed container, such as a resealable bag.
- Store the sealed container containing slides with fresh frozen tissue at -80°C for up to four weeks.

Store Slides in a Sealed Container



Xenium Slide Handling

- Always wear gloves when handling slides.
- The bottom of the slide is indicated by the etched label, which should be readable when in the proper position.
- The tissue sections should always be placed within the Sample Area on etched label side of the slide.
- Hold the slide on the label. DO NOT touch the tissue sections or near fiducials.
- Minimize exposure of the slides to sources of particles and fibers.
- Keep the slide cassette flat on the bench when adding reagents to the Sample Area.
- Ensure that no absorbent surface is in contact with the reagents on the slide during incubation.
- When pipetting reagent onto a slide, avoid generating bubbles. Avoid pipetting directly onto the tissue.



Xenium Cassette



- The Xenium Cassette is a single use item.
- The Xenium Cassette encases the slide and creates a leakproof well for adding reagents.
- Place the slide in the Xenium Cassette only when specified.
- Inner and outer tabs on the bottom half of the Xenium Cassette are used for holding the slide in the cassette. Applying excessive force to the cassette may cause the slide to break.
- The Xenium Cassette is assembled manually. See [Xenium Cassette Assembly & Removal](#) instructions for details.
- The Xenium Cassette includes an attached Xenium Gasket. The Xenium Gasket corresponds to the Sample Area on the slides.

- The etched slide label is visible in the label window when properly assembled.
- Ensure that the Xenium Cassette and gasket are free of debris prior to assembly. If placing the top half of the cassette on a surface, ensure the gasket faces up so it does not collect debris.
- Visually inspect the gasket to ensure it is seated properly. If the gasket appears warped, the Xenium Cassette is still safe to use as long as the cassette can fully close and no reagent leakage is observed.


Xenium Cassette Assembly

Ensure slide is completely dry before assembling into cassette. Visually inspect cassette and gasket prior to cassette assembly.




Exercise caution when handling slide edges to prevent injury.

Place top and bottom halves of cassette on bench

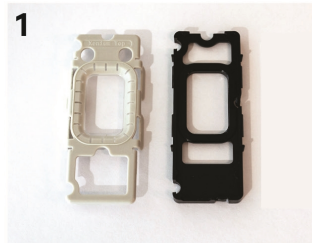


Place Xenium slide with tissue side facing upwards into bottom half of cassette; ensure label is toward bottom of cassette

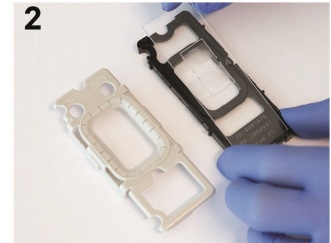

Press slide down into grooves of the bottom half of the cassette until it sits firmly in place



Secure clips of top half with tabs of bottom half (on both sides)

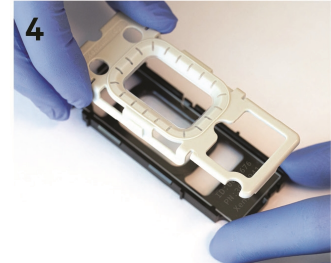

Apply even pressure on top of cassette until all clips click shut. Verify that clips are completely secured over tabs




Slides in images are representative.




Once cassette is assembled, DO NOT remove slide until after Xenium Analyzer imaging and decoding for optional H&E staining step.

Xenium Cassette Removal


Pull inner clips from inner tabs to detach top and bottom halves of cassette

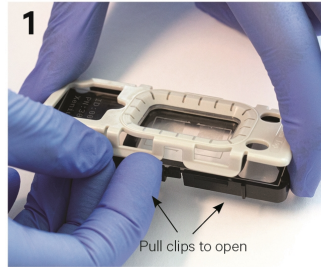

Open cassette by continuing to lift inner clips upward

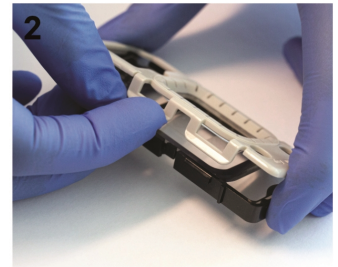


Hold slide by the label and lift slide out from bottom half

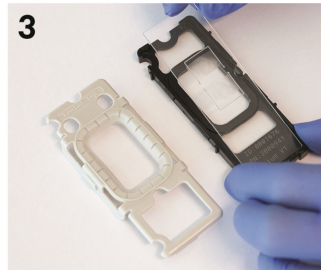

Slides in images are representative.

Reagent Addition to Wells

- Place assembled cassette flat on a clean work surface.
- Dispense and remove reagents along the side of the well without touching the tissue sections and without introducing bubbles.
- Always cover the Sample Area completely when adding reagents to the well. A gentle tap may help spread the reagent more evenly.

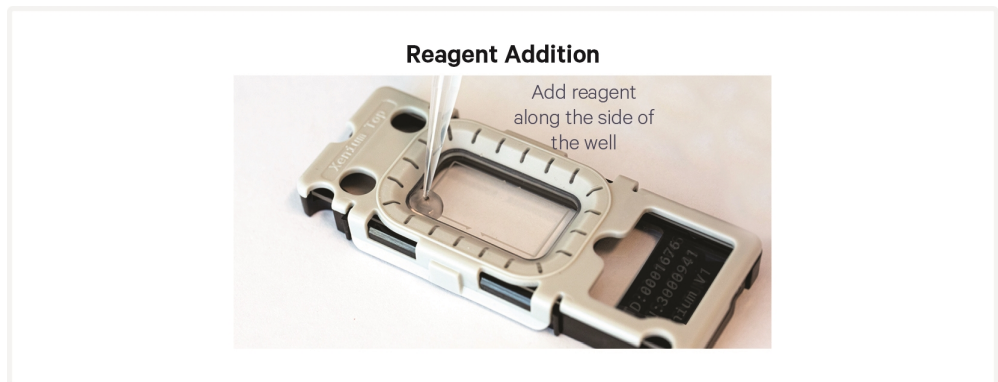

Reagent Removal from Wells

- Place assembled cassette flat on a clean work surface.
- Slightly tilt the cassette while removing the reagent.
- Place the pipette tip on the bottom edge of the well.
- Remove reagents along the side of the well without touching the tissue sections.
- Remove all liquid from the well in each step.




Xenium Cassette Lid Application & Removal

Application

- Place the Xenium Cassette flat on a clean work surface.
- Hold the Xenium Cassette Lid with index and middle finger on two upper tabs and thumb on the lower clip.
- Align the Xenium Cassette Lid with the surface of the Xenium Cassette. Hook the two upper clips into the two holes on the top of the cassette.
- Push the lid down until the lower clip clicks into place.
- Inspect the lid to confirm placement.

Removal

- Place the Xenium Cassette flat on a clean work surface.
- Push on the top of the two upper tabs with index and middle fingers.
- Use thumb to push in on the lower clip.
- While maintaining inward pressure, pull upward with thumb until the lower clip disengages.
- Ensure that no liquid splashes out of the well.

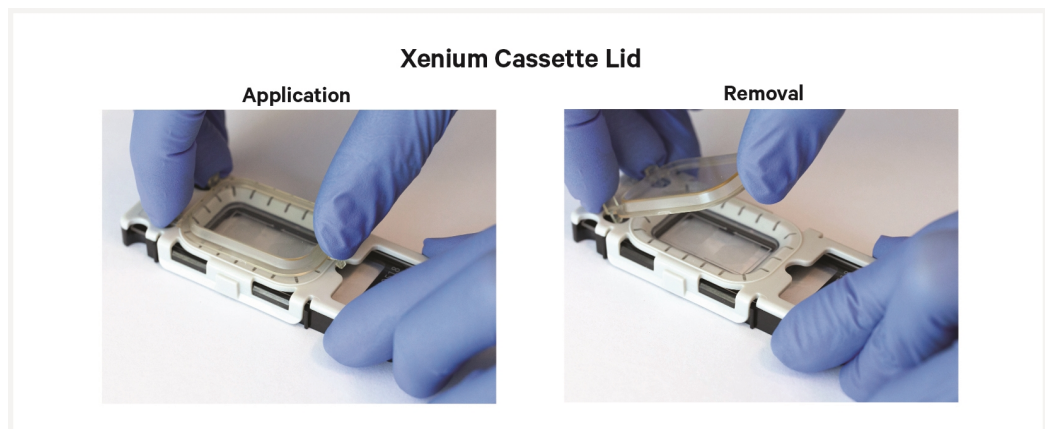


Note that Xenium Cassette Lids are a single use item and should be discarded after each use. PBS-T washes DO NOT require sealing of the cassette with a lid.

Slide Incubation Guidance

Incubation at a specified temperature

Incubation using a Thermal Cycler:

- Position a Xenium Thermocycler Adaptor on a thermal cycler that is set at the incubation temperature. Ensure thermal cycler has reached appropriate temperature prior to starting incubation.
- Ensure that the Thermocycler Adaptor is fully inserted into the thermal cycler and is in contact with the thermal cycler block surface uniformly.
- When incubating a slide, position the slide on the Thermocycler Adaptor with the tissue side facing up.
- Ensure the Sample Area is aligned with the corresponding area on the Thermocycler Adaptor. **DO NOT** close lid.
- When incubating a slide encased in a Xenium Cassette, place the assembled unit on the Thermocycler Adaptor with the well facing up. The cassette should always be sealed with a Xenium Cassette Lid when on the Thermocycler Adaptor unless indicated otherwise.

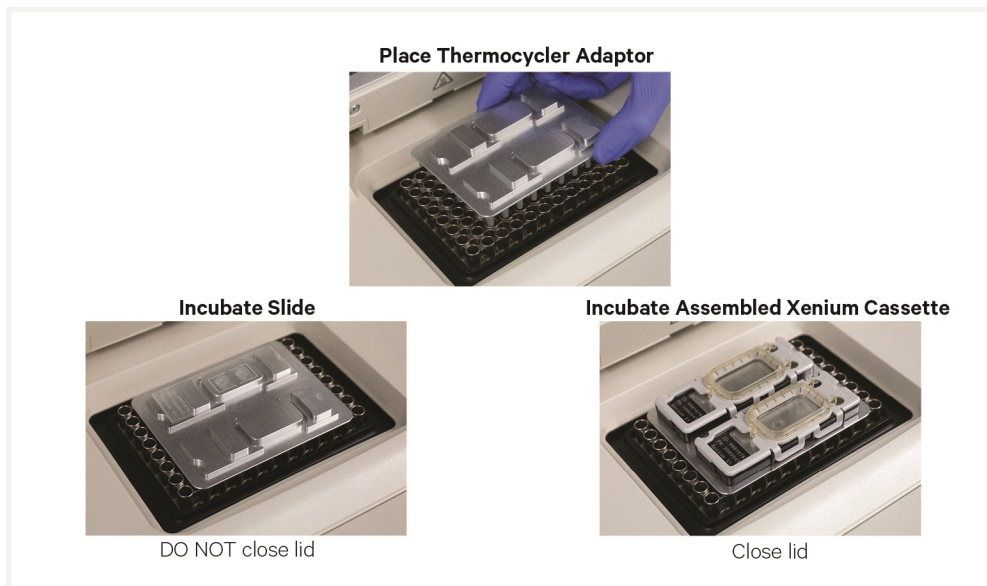

Incubation on ice

- Place Xenium slide(s) with label toward the top of the slide mailer for incubations on ice.
- Separate multiple slides by at least one slotted channel inside the mailer.
- Avoid placing slides in the last slotted channel of the mailer. Slides with tissues in the last position may get scratched if facing the mailer wall.
- Ensure slide mailer is submerged in the ice up to the lower part of the pink cap and is in standing position during incubation.

Incubation at room temperature

- Place Xenium slide(s) with label toward the top of the slide mailer for incubations at room temperature.
- Separate multiple slides by at least one slotted channel inside the mailer.
- Avoid placing slides in the first or last slotted channel of the mailer. Slides with tissues in the first or last position may get scratched if facing the mailer wall.
- Ensure the slide mailer is in standing position during incubation.

Tissue Detachment on Xenium Slides



- Monitor section adhesion on Xenium slides throughout the workflow.
- Tissue detachment during the workflow can negatively impact performance. If observed, contact support@10xgenomics.com.
- For more information, refer to Troubleshooting.

Protocol Steps & Timing

~2.5 hours

Steps	Timing	Stop & Store
Step 1 – Fixation & Permeabilization		
1.1 Preparation - Buffers	30 min	
1.2 Slide Preparation	5 min	
1.3 Fixation	30 min	
1.4 Permeabilization	65 min	
1.5 Cassette Assembly	10 min	




Note there are no safe stopping points during this workflow.


1. Fixation & Permeabilization

1.0 Overview

This chapter provides guidance on fixation and permeabilization of Xenium slides containing fresh frozen tissue sections.

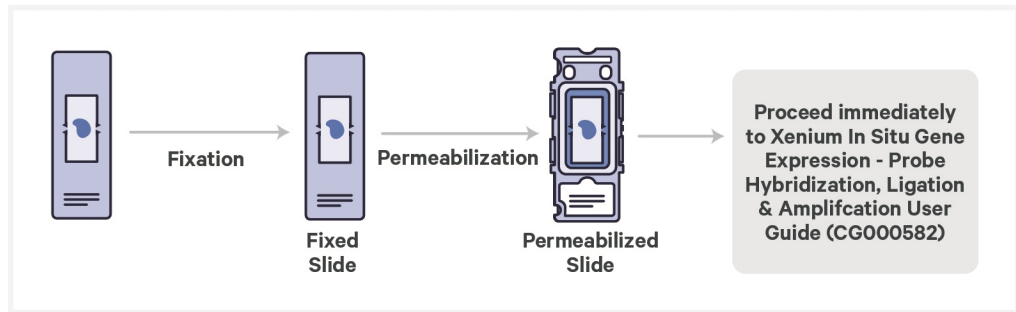

Protocol Overview

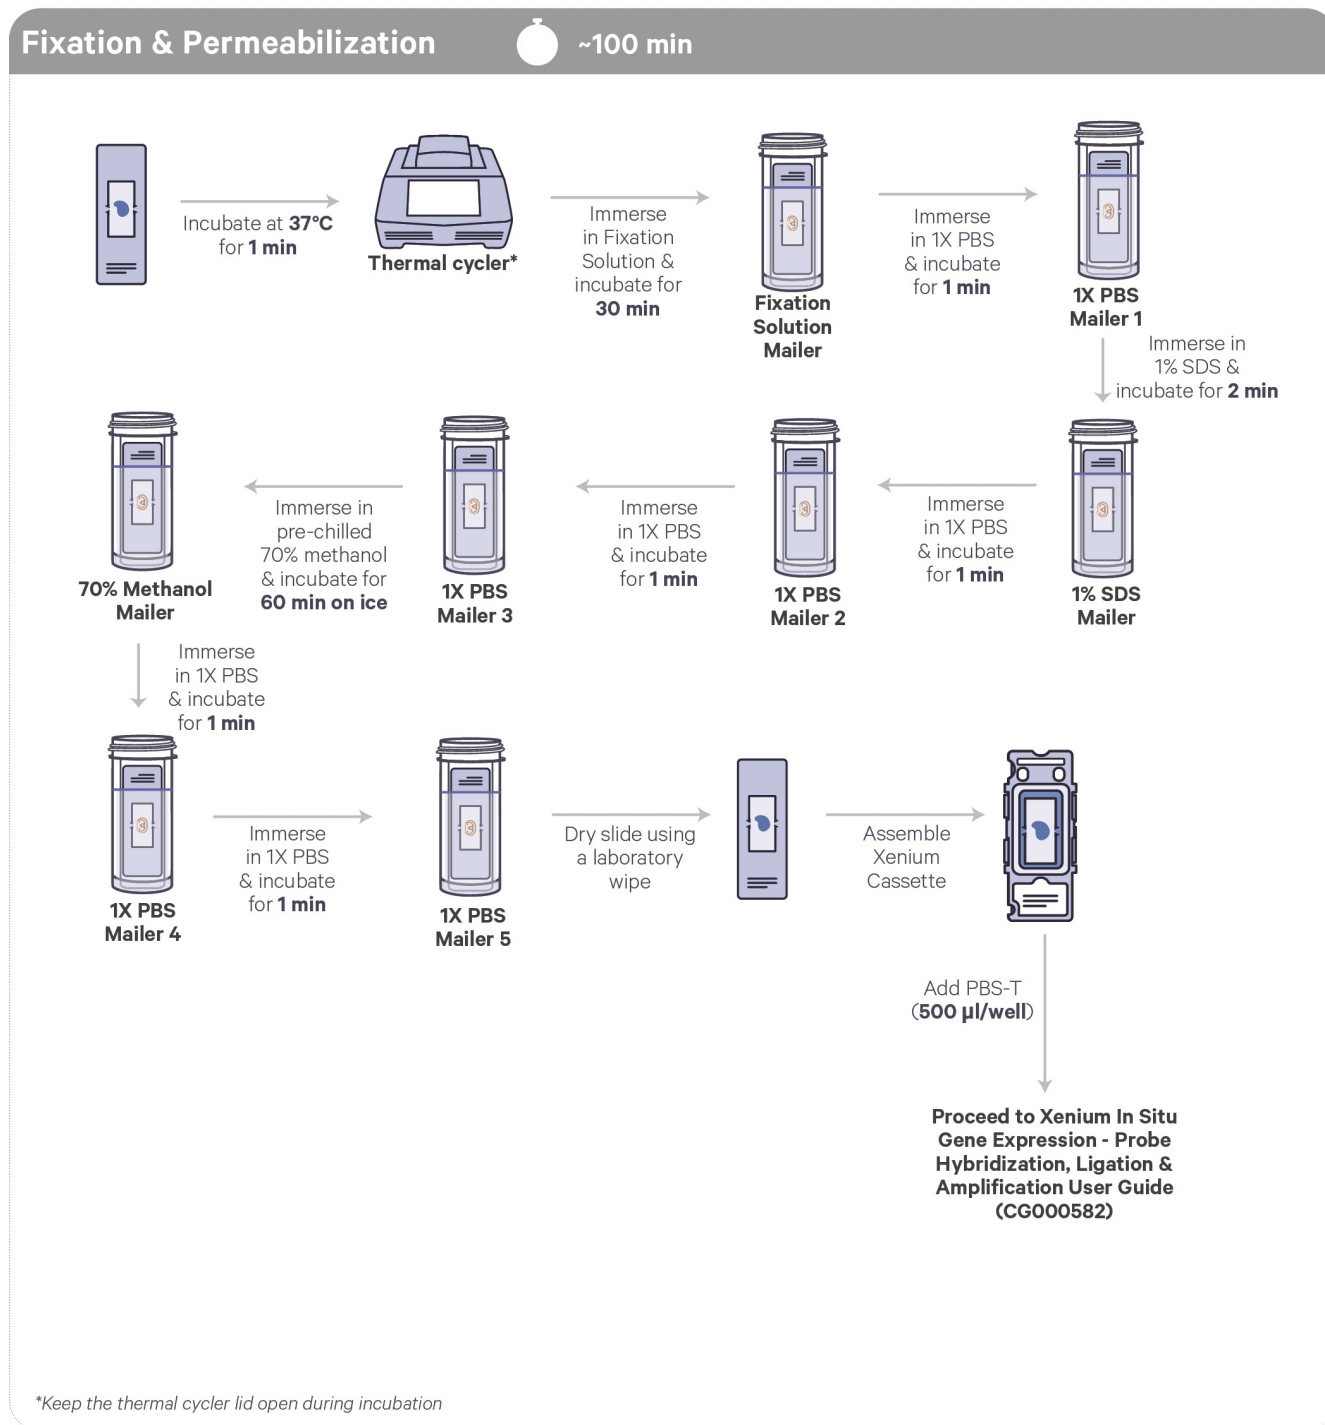

Get Started - Fixation & Permeabilization

Each 10x Genomics reagent tube is good for two Xenium Slides.

Fixation & Permeabilization Items	10x PN	Preparation & Handling	Storage	
Obtain				
<input type="checkbox"/>	Nuclease-free Water	-	-	Ambient
<input type="checkbox"/>	10X PBS	-	-	Ambient
<input type="checkbox"/>	Formaldehyde or Paraformaldehyde	-	-	Ambient
<input type="checkbox"/>	10% SDS	-	-	Ambient
<input type="checkbox"/>	Methanol	-	-	Ambient
<input type="checkbox"/>	10% Tween-20	-	-	Ambient
<input type="checkbox"/>	Slide Mailers	-	-	Ambient
<input type="checkbox"/>	Forceps	-	-	Ambient
<input type="checkbox"/>	Xenium Slides (2 pack) with fresh frozen tissue sections	3000941	Prepared according to Xenium In Situ for Fresh Frozen - Tissue Preparation Guide (CG000579).	-80°C

1.1 Preparation - Buffers

Prepare all buffers fresh according to the tables below before retrieving tissue sections from **-80°C**.



Prepare buffers in appropriate sized conical tube or bottle and transfer carefully to corresponding slide mailer.

- a. Prepare 1X PBS. Add reagents in the order listed. Invert gently to mix. Maintain at room temperature. This volume of 1X PBS is sufficient for washes in all subsequent steps of this Demonstrated Protocol.

1X PBS				
Items		Stock	Final	Total Amount (ml)
<input type="checkbox"/>	Nuclease-free water	-	-	63.0
<input type="checkbox"/>	RNase free PBS	10X	1X	7.0
<input type="checkbox"/>	Total	-	-	70.0

- b.** Using 1X PBS from step 1.1a, prepare Fixation Solution using either Formaldehyde or Paraformaldehyde according to the appropriate table below. Add reagents in the order listed. Invert gently to mix. Maintain at room temperature.

Fixation Solution (using Formaldehyde)				
Items		Stock	Final	Total Amount (ml)
<input type="checkbox"/>	1X PBS	-	-	9.0
<input type="checkbox"/>	Formaldehyde	37%	3.7%	1.0
<input type="checkbox"/>	Total	-	-	10.0

OR

Fixation Solution (using Paraformaldehyde)				
Items		Stock	Final	Total Amount (ml)
<input type="checkbox"/>	1X PBS	-	-	7.5
<input type="checkbox"/>	Paraformaldehyde	16%	4%	2.5
<input type="checkbox"/>	Total	-	-	10.0

- c.** Prepare 1% Sodium dodecyl sulfate (SDS). Verify no precipitate in SDS before use. Add reagents in the order listed. Invert gently to mix. Maintain at room temperature.

1% SDS				
Items		Stock	Final	Total Amount (ml)
<input type="checkbox"/>	Nuclease-free water	-	-	9.0
<input type="checkbox"/>	SDS (verify no precipitate)	10%	1%	1.0
<input type="checkbox"/>	Total	-	-	10.0


- d. Prepare 70% Methanol. Add reagents in the order listed. Invert gently to mix.

Pre-chill 70% Methanol on ice for **30 min** before starting Fixation protocol. Cap mailer and submerge in the ice up to the lower part of the pink cap.

70% Methanol				
Items		Stock	Final	Total Amount (ml)
<input type="checkbox"/>	Methanol	100%	70%	7.0
<input type="checkbox"/>	Nuclease-free water	-	-	3.0
<input type="checkbox"/>	Total	-	-	10.0

- e. Using 1X PBS from step 1.1a, prepare PBS-Tween (PBS-T). Add reagents in the order listed. Invert gently to mix. Maintain at room temperature. This volume of PBS-T is sufficient for washes in all subsequent steps of this Demonstrated Protocol.

PBS-T				
Items		Stock	Final	Total Amount (µl)
<input type="checkbox"/>	1X PBS	-	-	1,990
<input type="checkbox"/>	Tween-20	10%	0.05%	10
<input type="checkbox"/>	Total	-	-	2,000

 *Pipette Tween-20 slowly to fully dispense from pipette tip and to avoid formation of air bubbles.*

- f. Prepare eight total slide mailers for fixation.

For Fixation & Permeabilization		
Items (from 1.1a-1.1d)		Preparation & Handling
<input type="checkbox"/>	Fixation Solution	Label one slide mailer as Fixation Solution Mailer. Dispense 10 ml Fixation Solution.
<input type="checkbox"/>	1X PBS	Label five slide mailers as 1X PBS Mailer 1, 1X PBS Mailer 2, 1X PBS Mailer 3, 1X PBS Mailer 4, and 1X PBS Mailer 5. Dispense 10 ml 1X PBS in each.
<input type="checkbox"/>	1% SDS	Label one slide mailer as 1% SDS Mailer. Dispense 10 ml 1% SDS solution.
<input type="checkbox"/>	70% Methanol	Label one slide mailer as 70% Methanol Mailer. Dispense 10 ml 70% Methanol. Pre-chill 70% Methanol on ice for 30 min.

1.2 Slide Preparation

- a. Place Xenium Thermocycler Adaptor in thermal cycler set to incubate at **37°C**. DO NOT close the lid.


Ready the Fixation Solution Mailer and a timer set to 1 min, which are needed in the following steps.

- b. Prepare an ice bucket of dry ice.
- c. Remove slide mailer containing stored fresh frozen tissue slide(s) from **-80°C** and bury into the dry ice.



*Alternatively, submerge an uncapped empty slide mailer in dry ice and incubate for **5 min**. Remove slides from **-80°C** storage with a pair of forceps and immediately place in pre-chilled empty slide mailer on dry ice.*

- d. Using a pair of slide forceps, move the slide(s) from dry ice to the **37°C** pre-heated thermal cycler for **1 min**. Place slide on the Thermocycler Adaptor with the tissue side facing up. Ensure the Sample Area is aligned with the corresponding area on the Thermocycler Adaptor. DO NOT close the lid.

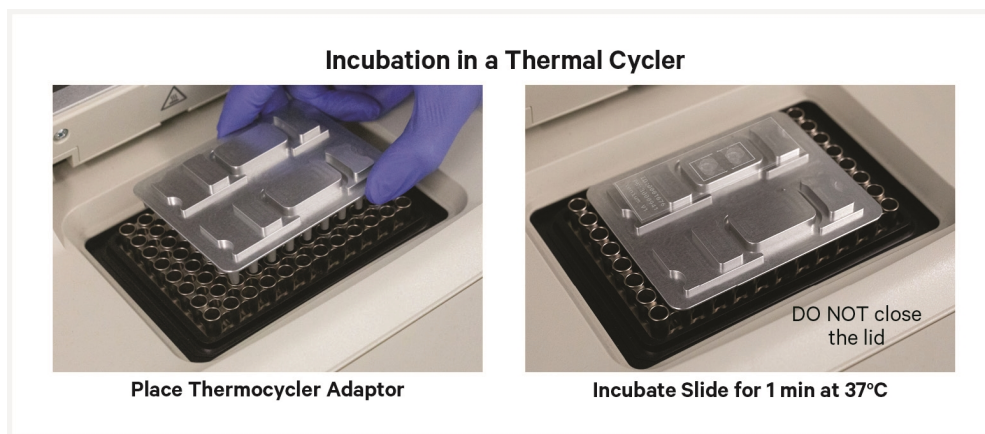


1.3 Fixation

- a. **Immediately** remove slide from thermal cycler following incubation. Gently immerse slide in the Fixation Solution Mailer using slide forceps and incubate for **30 min** at **room temperature**.



Formaldehyde and Paraformaldehyde should be handled in a biosafety hood due to their hazardous nature. Transfer slides immediately to Fixation Solution following removal from thermal cycler to prevent formation of freezing artifacts on the slides.

See [Tips & Best Practices](#) for guidance on properly immersing slides into mailers.

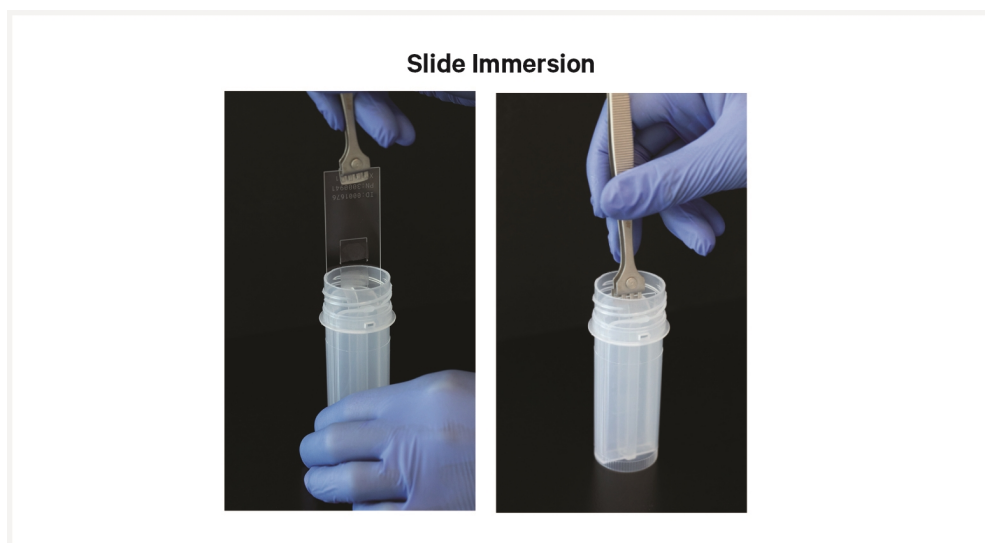

Ensure 70% Methanol Mailer is pre-chilled on ice before proceeding to next step.

1.4 Permeabilization



Start thawing reagents for Probe Hybridization during Permeabilization as indicated in the Xenium In Situ Gene Expression - Probe Hybridization, Ligation & Amplification User Guide (CG000582).

- a. Gently immerse slide in the 1X PBS Mailer 1 and incubate for **1 min** at **room temperature**.

Remove any marker annotations on slide using a lint-free laboratory wipe and 100% Ethanol.

- b. Gently immerse slide in the 1% SDS Mailer and incubate for **2 min** at **room temperature**.
- c. Gently immerse slide in the 1X PBS Mailer 2 and incubate for **1 min** at **room temperature**.
- d. Gently immerse slide in the 1X PBS Mailer 3 and incubate for **1 min** at **room temperature**.
- e. Gently immerse slide in the pre-chilled 70% Methanol Mailer and incubate for **60 min** on **ice**. Cap mailer and fully submerge in the ice up to the lower part of the pink cap.

Methanol Incubation



- f. Gently immerse slide in the 1X PBS Mailer 4 for **1 min** at **room temperature**.
- g. Gently immerse slide in the 1X PBS Mailer 5 for **1 min** at **room temperature**.
- h. Remove slide from the 1X PBS Mailer 5.

1.5 Cassette Assembly

- a. Remove any remaining 1X PBS from the slide using a lint-free laboratory wipe. Dry back of slide completely and front of slide outside of Sample Area without touching or damaging the tissue sections. Place the slide in the Xenium Cassette.



Refer to [Tips & Best Practices](#) for guidance on Xenium Cassette Assembly. Work quickly to avoid drying out of tissue sections.

- b. Add **500 µl** 1X PBS-T.




Optional: photograph the slide against a black background. This image can be used for comparison purposes to identify tissue detachment downstream in the workflow. Work quickly as this is not a safe stopping point. See [Troubleshooting](#) for more details.



- c. Proceed **immediately** to Xenium In Situ Gene Expression - Probe Hybridization, Ligation & Amplification User Guide (CG000582).

Assembled Xenium Cassette

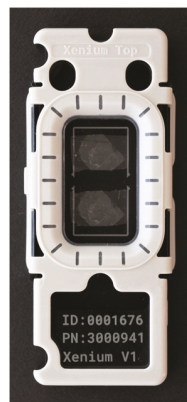

Troubleshooting

Tissue Detachment on Xenium Slides

Tissue sections may detach from Xenium slides during on-slide workflows. Tissue adhesion to the slide is impacted both by tissue processing and tissue quality.

Careful tissue preparation is critical for adhesion in on-slide workflows. Consult Xenium In Situ for Fresh Frozen - Tissue Preparation Guide (Document CG000578) for tissue QC and sectioning best practices. Below are some additional best practices for minimizing detachment during on-slide workflows:

- Do not pipette directly onto the tissue.
- Gently add and remove reagents from the well. Forceful addition or removal of reagents can agitate tissue and lead to detachment.
- Avoid touching in and around the Sample Area of the Xenium slide.
- Work quickly and carefully during reagent addition and removal.

In addition to following best practices, it is possible to monitor section adhesion on Xenium slides throughout the workflow. Taking a photograph of the slide at the beginning of the on-slide workflow and comparing with post-assay workflow images can help identify whether tissue shape has changed significantly, an indication of detachment. Steps when slide photos can be taken are noted in the protocol. These QC images can be compared with the DAPI overview scan as part of the Web Summary file to see whether tissue morphology has changed in the workflow.

If tissue detachment occurs, send pictures to support@10xgenomics.com for further assistance.

Cassette Assembly Failure

Incorrect assembly of the Xenium Cassette with a Xenium slide can negatively impact assay performance. Always dry the front and the back of the slide completely using a lint-free laboratory wipe while avoiding touching or damaging of the tissue sections. Inspect the slide carefully to ensure it is seated fully within the cassette before assembly. Additionally, inspect gasket prior to assembly to ensure it is not damaged or leaking.

Example scenarios that may indicate incorrect Xenium Cassette assembly are described below:

- If a gap appears between the two halves of the cassette after assembly.
- If the cassette does not click shut or appears domed after assembly.
- If the Xenium Thermocycler Adaptor is wet following removal from the thermal cycler, indicating reagent leakage from the cassette.


If the cassette is incorrectly assembled, disassemble and reassemble the cassette as instructed in [Tips & Best Practices](#).

Incorrect cassette assembly as indicated by a gap between the two halves of the cassette

Correct cassette assembly



Incorrect cassette assembly

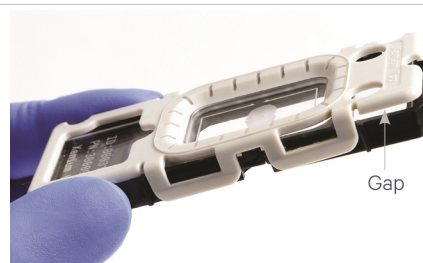

Document Revision Summary

Document Number	CG000581
Title	Xenium In Situ for Fresh Frozen – Fixation & Permeabilization Demonstrated Protocol
Revision	Rev C
Revision Date	August 2023
Specific Changes	<p>Removed Veriti 96-well Thermal Cycler (Thermo Fisher Scientific) from Recommended Thermal Cyclers list (page 5).</p> <p>Added 10% Tween-20 (Bio-Rad) to Specific Reagents & Consumables list (page 7).</p> <p>Updated cassette handling guidance in Tips & Best Practices (page 15).</p> <p>Added optional photograph guidance (pages 31 -32).</p> <p>Updated Cassette Assembly Failure guidance (page 33).</p>
General Changes	Updated for general minor consistency of language and terms throughout.

© 2023 10x Genomics, Inc. (10x Genomics). All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third-party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. A non-exhaustive list of 10x Genomics' marks, many of which are registered in the United States and other countries can be viewed at: www.10xgenomics.com/trademarks. 10x Genomics may refer to the products or services offered by other companies by their brand name or company name solely for clarity, and does not claim any rights in those third-party marks or names. 10x Genomics products may be covered by one or more of the patents as indicated at: www.10xgenomics.com/patents. The use of products described herein is subject to 10x Genomics Terms and Conditions of Sale, available at www.10xgenomics.com/legal-notice, or such other terms that have been agreed to in writing between 10x Genomics and user. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

The use of 10x Genomics products in practicing the methods set forth herein has not been validated by 10x Genomics, and such non-validated use is NOT COVERED BY 10X GENOMICS STANDARD WARRANTY, AND 10X GENOMICS HEREBY DISCLAIMS ANY AND ALL WARRANTIES FOR SUCH USE. Nothing in this document should be construed as altering, waiving or amending in any manner 10x Genomics terms and conditions of sale for the Chromium Controller or the Chromium Single Cell Controller, consumables or software, including without limitation such terms and conditions relating to certain use restrictions, limited license, warranty and limitation of liability, and nothing in this document shall be deemed to be Documentation, as that term is set forth in such terms and conditions of sale. Nothing in this document shall be construed as any representation by 10x Genomics that it currently or will at any time in the future offer or in any way support any application set forth herein.

Contact:

Email: support@10xgenomics.com
10x Genomics
6230 Stoneridge Mall Road
Pleasanton, CA