

Xenium In Situ for FFPE – Tissue Preparation Guide

Introduction

Xenium In Situ for FFPE is designed to measure mRNA in tissue sections derived from formalin fixed & paraffin embedded (FFPE) tissue samples and requires a Xenium slide with intact tissue sections as input. Proper tissue handling, storage, and preparation techniques preserve the morphological quality of tissue sections and integrity of mRNA transcripts.

This Tissue Preparation Guide provides guidance on:

- Tissue fixation and embedding.
- Best practices for handling tissue samples and Xenium slides before and after sectioning.
- DAPI and Hematoxylin and Eosin (H&E) staining to check tissue quality.
- Sectioning and tissue placement practice.
- Sectioning of tissue samples and placement of sections on Xenium slides.

Additional Guidance

Refer to the 10x Genomics Support website for additional resources. This protocol is compatible with both Xenium In Situ (referred to as Xenium v1) and Xenium Prime In Situ reagents and downstream assay workflows as specified in the table.

Compatible Reagent Kits & Downstream Workflows		
	Xenium v1	Xenium Prime
Assay	Xenium In Situ Gene Expression (CG000582)	Xenium Prime In Situ Gene Expression with optional Cell Segmentation Staining (CG000760)
Workflows	Xenium In Situ Gene Expression with Cell Segmentation Staining (CG000749)	

Contents

Introduction

Xenium In Situ Gene Expression Reagent Kits	4
Xenium Prime In Situ Gene Expression Reagent Kits	6
Recommended Thermal Cyclers	7
Specific Reagents & Consumables	8
Xenium Slide	11

Tissue Handling, Fixation, and Embedding Guidelines

Tips & Best Practices

Icons	17
Sample Preparation	17
Sectioning Speed	17
Section Thickness	17
Water Bath Temperature & Section Floating Time	17
Xenium Slide Template	18
Section Placement on Xenium Slides	19
Optional Tissue Trimming & Scoring	21
Tissue Detachment on Xenium Slides	21
Handling Xenium Slides	22
Xenium Slide Incubation	22

1. FFPE Tissue Sectioning, Section Placement, and Quality Assessment

Overview	24
1.0 Get Started	27
1.1 Facing the Block	28
1.2 Sectioning	29
1.3 Section Placement on Blank Slides	31
1.4 Deparaffinization & Quality Assessment	33
1.5 DAPI Quality Assessment	33
1.6 H&E Tissue Quality Assessment	34
DV200 Performance and Recommendations	34

2. Optional - Practice FFPE Tissue Sectioning & Section Placement

Overview	36
2.0 Get Started	37

3. FFPE Tissue Sectioning & Section Placement

Overview	38
3.0 Get Started	40
3.1 Section Placement on Xenium Slides	41

Troubleshooting

Appendix

Deparaffinization & Quality Assessment	47
Deparaffinization	50
DAPI Staining	52
Coverslipping	52
Coverslip Removal	53
H&E Staining	56
Coverslipping	58
Shipping Guidance	63
RNA Quality Assessment of FFPE Tissue Block	63
References	64

Document Revision Summary

Introduction


Xenium In Situ Gene Expression Reagent Kits

Compatible only with the following Xenium v1 workflows:

- Xenium In Situ Gene Expression (CG000582)
- Xenium In Situ Gene Expression with Cell Segmentation Staining (CG000749)

Refer to SDS for handling and disposal information.

Xenium Slides & Sample Prep Reagents (2 slides, 2 rxns) PN-1000460

Xenium Slides & Sample Prep Reagents			
(2 slides, 2 rxns), PN-1000460			
Store at -20°C			
		#	PN
	Xenium Probe Hybridization Buffer	1	2000390
	Xenium Post Hybridization Wash Buffer	1	2000395
	Xenium Ligation Buffer	1	2000391
	Xenium Ligation Enzyme A	1	2000397
	Xenium Ligation Enzyme B	1	2000398
	Xenium Amplification Mix	1	2000392
	Xenium Amplification Enzyme	1	2000399
	Reducing Agent B	1	2000087
	Xenium Autofluorescence Mix	1	2000753
	Xenium FFPE Tissue Enhancer*	1	2000798
	Xenium Nuclei Staining Buffer	1	2000762
	Perm Enzyme B	1	3000553
	Xenium Slides (2 pack)	1	3000941


10x
GENOMICS

Only the Xenium Slides (2 pack) are needed for this workflow.

**The reagent name may or may not include the prefix "Xenium"; Irrespective of the prefix, the indicated part number is associated with the reagent name.*

Xenium Slides Kit (4 slides) PN-1000659

Xenium Slides Kit (2 slides), PN-1000659 Store at -20°C		
	#	PN
Xenium Slides (2 pack)	2	3000941



Xenium Slides Kit (16 slides) PN-1000660

Xenium Slides Kit (2 slides), PN-1000660 Store at -20°C		
	#	PN
Xenium Slides (2 pack)	8	3000941



Purchase the Xenium Slides Kit (4 or 16 slides) for additional slides as needed.

Xenium Prime In Situ Gene Expression Reagent Kits

Compatible only with the following Xenium Prime workflows:


- Xenium Prime In Situ Gene Expression with optional Cell Segmentation Staining (CG000760)

Refer to SDS for handling and disposal information.

Xenium Prime Sample Preparation Reagents with Slides - (2 rxns) PN-1000741

Contains Xenium Slides (2 pack) PN-1000465 and Xenium Prime Sample Preparation Reagents (2 rxns) PN-1000720. Only the slide kits are shown below, as the sample preparation reagents are not used in this protocol.

Xenium Slides Kit (2 slides), PN-1000465 Store at -20°C		
	#	PN
Xenium Slides (2 pack)	1	3000941



Xenium Prime Sample Preparation Reagents with Cell Segmentation with Slides - (2 rxns) PN-1000742

Contains Xenium Slides (2 pack) PN-1000465, Xenium Cell Segmentation Staining Reagents (2 rxns) PN-1000661, and Xenium Prime Sample Preparation Reagents (2 rxns) PN-1000720. Only the slide kits are shown below, as the sample preparation reagents are not used in this protocol.

Xenium Slides Kit (2 slides), PN-1000465 Store at -20°C		
	#	PN
Xenium Slides (2 pack)	1	3000941



Recommended Thermal Cyclers

Xenium v1 validated thermal cyclers:

Supplier	Description	Part Number
Bio-Rad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module (discontinued)	1851197
Analytik Jena	Biometra TAdvanced 96 SG with 96-well block (silver, 0.2 mL) and gradient function	846-x-070-241 (<i>where x=2 for 230 V; 4 for 115 V; 5 for 100 V, 50-60 Hz</i>)
VWR	Gradient thermal cycler, XT ⁹⁶ Gradient, with 96-well gradient block and standard lid	76452-153
Marshall Scientific	MJ Research PTC-200 Thermal Cycler (discontinued)	05434-05

Xenium Prime validated thermal cyclers:

Supplier	Description	Part Number
Bio-Rad	C1000 Touch Thermal Cycler with 96-Deep Well Reaction Module (discontinued)	1851197
Bio-Rad	PTC Tempo Deepwell Thermal Cycler	12015392
Analytik Jena	Biometra TAdvanced 96 SG with 96-well block (silver, 0.2 mL) and gradient function	846-x-070-241 (<i>where x=2 for 230 V; 4 for 115 V; 5 for 100 V, 50-60 Hz</i>)
ThermoFisher Scientific	VeritiPro 96-well Thermal Cycler	A48141

Specific Reagents & Consumables

The listed items have been tested by 10x Genomics and perform optimally with the assay. **Substituting materials may adversely affect system performance.** For items with multiple options listed, choose option based on availability and preference. Refer to the manufacturer's website for regional part numbers.

For FFPE Tissue Sectioning & Section Placement				
	Item	Alternatives/Options	Vendor	Part Number
<input type="checkbox"/>	Microtome	EpreDia HM 355S Automatic Microtome <i>Or any standard histology grade microtome</i>	Fisher Scientific	23-900-672
<input type="checkbox"/>	Microtome blade	EpreDia MX35 Premier Disposable Microtome Blades, Low Profile	Fisher Scientific	3052835
<input type="checkbox"/>	Cool-Cut <i>(optional)</i>	Thermo Scientific Cool-Cut <i>(optional)</i>	Fisher Scientific	77-112-0
<input type="checkbox"/>	Section transfer system (STS) <i>(optional)</i>	Thermo Scientific Section Transfer System (STS), <i>Optional - If using Section Transfer System</i>	Fisher Scientific	771200
<input type="checkbox"/>	Probes	Fisherbrand Fine Precision Probe	Fisher Scientific	12-000-153
<input type="checkbox"/>	Forceps	Fisherbrand Curved Medium Point General Purpose Forceps	Fisher Scientific	16-100-110
<input type="checkbox"/>	Blank Slides <i>(optional, for sectioning practice)</i>	Superfrost Plus Microscope Slides	Fisher Scientific	12-550-15
<input type="checkbox"/>	Water bath	Tissue Floating Bath, Lighted <i>Or any equivalent water bath</i>	Geyer	194242
		EpreDia Digital Round Tissue Section Water Bath <i>if using optional Section Transfer System</i>	Fisher Scientific	A84600061
<input type="checkbox"/>	Section dryer oven <i>(optional, but recommended)</i>	EpreDia High Capacity Section Dryer	Fisher Scientific	A84600051
<input type="checkbox"/>	Brushes	Camel Hair Brushes <i>or any equivalent paintbrush</i>	Ted Pella	11859
<input type="checkbox"/>	Fan <i>(optional, but recommended)</i>	Personal Rechargeable Fan <i>or any equivalent fan</i>	Holmes	085-01-0117
<input type="checkbox"/>	Cutting Mat	WellTech Cutting Mat	WellTech Precision Lab	N/A
<input type="checkbox"/>	Wax Trimmer <i>(optional)</i>	Electronic Microscopy Sciences Paraffin Block Trimmer Wax Trimmer, 115 VAC	Fisher Scientific	NC0310844
<input type="checkbox"/>	Marker <i>(optional)</i>	StatMark Pen	EMS	72109-12
Additional Materials				
<input type="checkbox"/>	Razor blades		-	-
<input type="checkbox"/>	Ultrapure/Milli-Q Water for Water Bath, <i>from Milli-Q Integral Ultrapure Water System or equivalent</i>		-	-

For Deparaffinization				
Item		Description	Vendor	Part Number
<input type="checkbox"/>	Xylene or Neo-clear	Xylene, Reagent Grade	Millipore Sigma	214736
		Xylene, Histological Grade	Millipore Sigma	534056
		Neo-clear Xylene Alternative Substitute <i>Only tested for the Xenium Gene Expression workflow</i>	Millipore Sigma	1098435000
<input type="checkbox"/>	Ethanol	Ethyl Alcohol, 200 Proof, anhydrous	Millipore Sigma	E7023
		Ethanol absolute ≥99.5%, TechniSolv, pure (Europe)	VWR	83813.360DP
<input type="checkbox"/>	Nuclease-free Water	Nuclease-free Water (not DEPC-treated)	Thermo Fisher Scientific	AM9932/ AM9937
<input type="checkbox"/>	Staining jar/dishes	Coplin Jar	VWR	100500-232
		Staining Dishes	VWR	25608-906
<input type="checkbox"/>	Section dryer oven	Epredia High Capacity Section Dryer <i>(Or equivalent. Thermal cyclers may also be used for section drying).</i>	Fisher Scientific	A84600051
Additional Materials				
<input type="checkbox"/>	Water bath or Thermomixer with 2 ml adapter			
<input type="checkbox"/>	Thermal Cyclers <i>(see Recommended Thermal Cyclers)</i>			
<input type="checkbox"/>	Slide drying rack			
<input type="checkbox"/>	Fume Hood			
<input type="checkbox"/>	Vortex			
For H&E Staining				
Item		Description	Vendor	Part Number
<input type="checkbox"/>	Hematoxylin	Hematoxylin Solution, Mayer's	Sigma Aldrich	MHS16
<input type="checkbox"/>	Eosin	Eosin Y Solution, Alcoholic	Leica	3801615
<input type="checkbox"/>	Bluing Reagent	Bluing Solution	Dako	CS702
<input type="checkbox"/>	Mounting Media	Surgipath SUB-X Mounting Media (discontinued)	Leica	3801741
		Cytoseal Mountant; 60, 280 and XYL	Fisher Scientific	22-050-262
<input type="checkbox"/>	Ethanol	Ethyl Alcohol, 200 Proof, anhydrous	Millipore Sigma	E7023
		Ethanol absolute ≥99.5%, TechniSolv, pure (Europe)	VWR	83813.360DP
<input type="checkbox"/>	Xylene	Xylene, Reagent Grade	Millipore Sigma	214736
		Xylene, Histological Grade	Millipore Sigma	534056

For H&E Staining				
<input type="checkbox"/>	Forceps	Tweezers, 4' Water Handling	Excelta Corp	491P-SA-PI
<input type="checkbox"/>	Filter Paper	Fisherbrand Qualitative Grade Plain Filter Paper Circles	Fisher Scientific	09-795-H
<input type="checkbox"/>	Coverslips	Fisherbrand Cover Glasses: Rectangles	Fisher Scientific	12-544-EP
		Cover Glasses, Rectangles	VWR	16004-322
Additional Materials				
<input type="checkbox"/>	Vortex			
<input type="checkbox"/>	Staining jar/dishes			
<input type="checkbox"/>	Wide-bore pipette tips			
<input type="checkbox"/>	Ultrapure/Milli-Q Water <i>from Milli-Q Integral Ultrapure Water System or equivalent</i>			




The instructions apply to both Xenium v1 and Xenium Prime assays. The consumables are referred to generically without always citing the version suffix. Based on the assay choice, always ensure that either Xenium v1 or Xenium Prime specific reagents and consumables are used.

Xenium Slide

- Xenium slides include an imageable area outlined by a white line measuring 12 mm x 24 mm, with an available sample positioning area measuring 235 mm² (10.45 mm x 22.45 mm). The available sample positioning area will be referred to as the Sample Area for the remainder of this document.
- The Sample Area is surrounded by fiducials. Tissue sections are placed within the Sample Area without obstructing the fiducials. The imageable area includes the area within the fiducial frame + Sample Area.
- The Sample Area can accommodate as many tissue sections as can fit within the space. Ensure tissue sections (including wax) DO NOT overlap.
- An etched label denoting the Slide ID, Part, and Version numbers is located at the bottom of the slide. Tissue sections should be placed on labeled-side of slide.

The Xenium Slide (PN-3000941) may not always include the suffix v1 in the etched label.

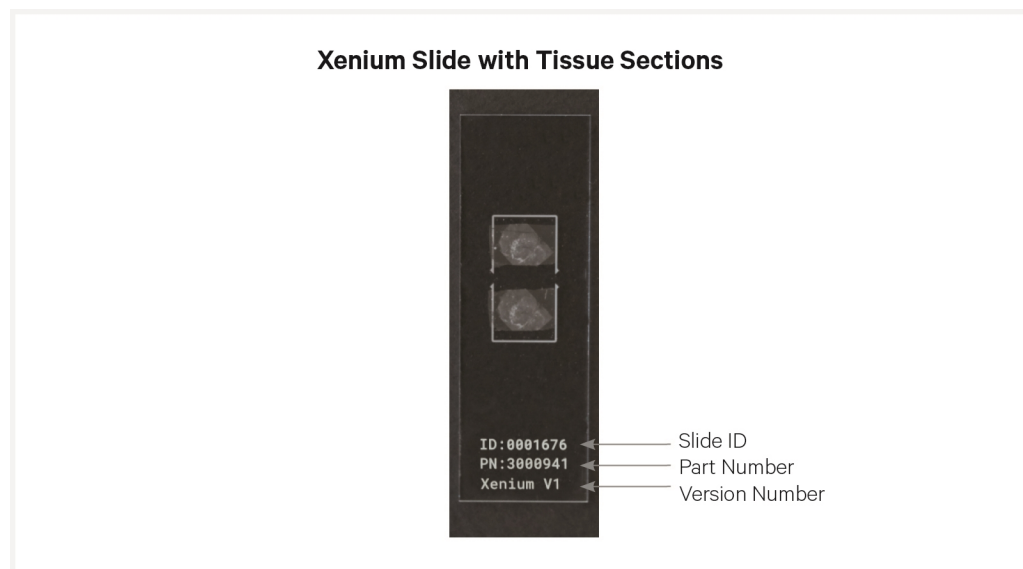

Tissue Handling, Fixation, and Embedding Guidelines

Tissue Handling


Prior to fixation and embedding, tissues should be handled according to the following guidelines to maximize RNA quality and prevent degradation.

Gentle Handling


Tissues should be handled gently to avoid mechanical stress. Mechanical stress may damage tissue structure and prevent proper fixation. Examples of processes that introduce mechanical stress include ischemia, coagulative necrosis from electrocautery, and haemorrhages from surgical trauma.

Minimizing Ischemia/Post Mortem Interval (PMI) and Fixation Timing

Prolonged ischemia and PMI can negatively affect tissue quality. If processing delays occur, store tissues in an isotonic solution and avoid exceeding four hours between tissue resection and fixation, though this time may be tissue-dependent. The images below show the negative effect of prolonged ischemia on RNA density.

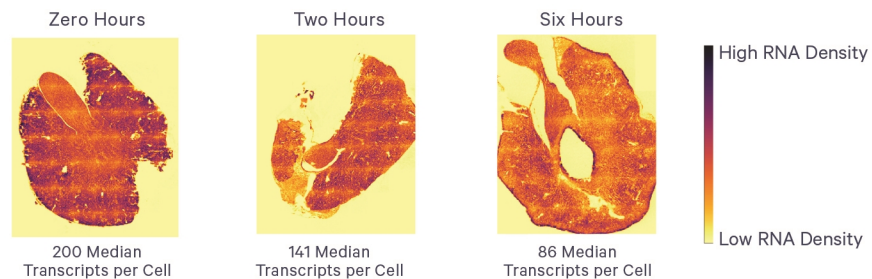

Delayed tissue fixation may lead to autolysis, degrading tissue and negatively impacting results. Tissue samples should be fixed immediately after resection.

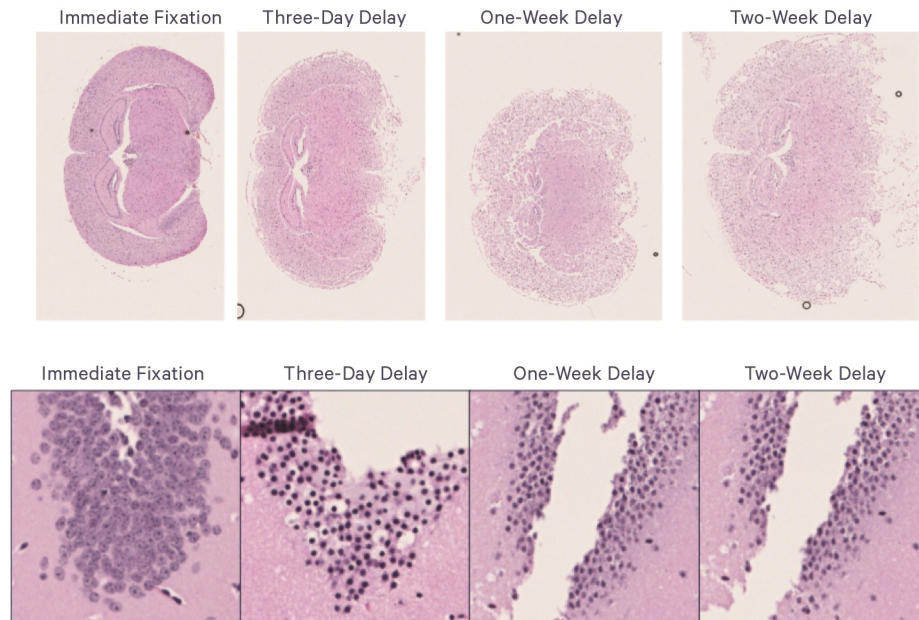

Tissue Storage

Store tissues in a cool and moist environment to prevent tissue drying and degradation. Tissues can be kept in an isotonic solution (e.g. RNase-free PBS) if tissue cannot be fixed immediately. Keeping tissues in isotonic solutions is not suitable for long-term storage. Avoid exceeding four hours. 10x Genomics cannot provide specific guidance on isotonic solutions or RNA preservation products.


Tissue Fixation and Embedding Guidelines

Prior to sectioning, tissues should be fixed and embedded according to the following guidelines to maximize RNA quality and prevent degradation. These steps generate a formalin fixed & paraffin embedded block that is ready for sectioning.


Optimizing Fixation Time

Under or overfixation of tissues can negatively impact assay performance. Fixation time may need optimization for specific organisms, tissue types, and disease states.

Underfixing tissues may result in the continued activities of some enzymes after tissue resection, which may cause degradation of proteins, nucleic acids, and lipids. RNA may also not be properly preserved in underfixed tissues. Lastly, underfixation can lead to tissue artifacts such as irregular chromatin patterns, overstained cytoplasm (eosin), and common autolysis artifacts such as separation of the epithelium from connective tissue. The images below show the negative impacts of underfixation in mouse liver on RNA density. Note the RNA density gradient that begins at the edge of the tissue.

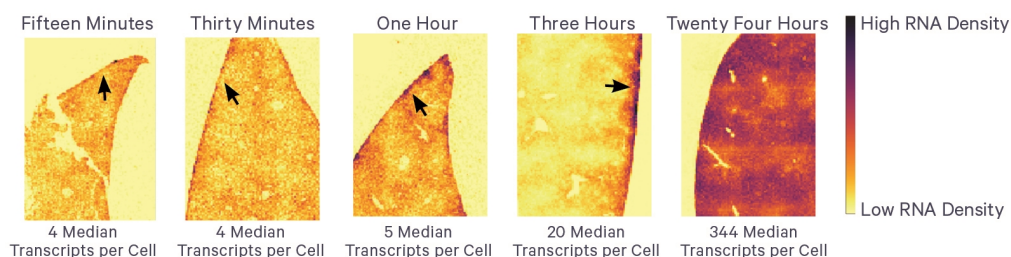

Overfixation may lead to a loss of structural integrity of certain molecular features, lipid oxidation, excessive crosslinking, and decreased antigenicity. Additionally, overfixation may make sectioning more challenging due to tissue hardening. Overfixation can lead to tissue artifacts such as irregularly shaped/smaller cells or hyperchromatic nuclei staining. The images below show structural effects of overfixation in mouse kidney, as well as the negative impact of overfixation on RNA density.

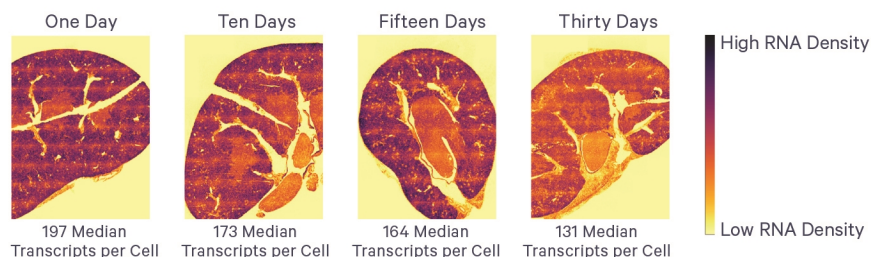

To avoid under or overfixation, consider the following:

Tissue Size

The thickness of the tissue significantly affects fixative penetration. Tissue sections should be no larger than a standard tissue cassette and no thicker than 5 mm.

Fixative and Fixative to Tissue Ratio

The use of 10% Neutral Buffered Formalin (NBF) at a fixative to tissue ratio of 20:1 is recommended for optimal performance.

Fixation Time and Temperature

Fixation should be carried out at 4°C for ~16-24 h to ensure proper fixative penetration. Fixation time may be tissue-dependent and require optimization. Ensure tissue is completely submerged and introduce light agitation.

Optimizing Embedding

Dehydration

After fixation, tissues are dehydrated in an ethanol series to displace any water remaining in the tissue. Inadequate dehydration may result in poor preservation of tissue structure and damage during sectioning.

Clearing

Tissues are "cleared" using a solvent to remove any remaining ethanol. Inadequate clearing may lead to poor wax infiltration, which can result in hard and brittle blocks that are difficult to section.

Infiltration

After clearing, wax is applied to the tissue and allowed to infiltrate. Inadequate wax infiltration may result in holes or gaps in the final block, which may lead to sectioning difficulties. Typically, wax is melted at 60–62°C prior to adding to the tissue. It is then allowed to cool to 20°C. Avoid excessive heat and check temperatures regularly during embedding. Use a high-quality wax with a low melting temperature.

Embedding

Finally, tissues are embedded in paraffin. Record orientation of the tissue during paraffin embedding to ensure proper spatiality for downstream region selection and analysis.

Additional Tips and Best Practices

- Regularly replace reagents used during the fixation and embedding process.
- DO NOT store or leave sample in fixative for an extended period of time, which will lead to overfixation
- Proceed immediately from fixation to dehydration, clearing, and embedding. If proceeding to dehydration immediately is not possible, transfer tissue from fixative to 70% ethanol for short-term storage.
- Store FFPE blocks properly to maintain integrity. Avoid exposure to high temperatures or humidity. For optimal storage, store at 4°C.

Tips & Best Practices

Icons



Tips & Best Practices section includes additional guidance



Signifies critical step requiring accurate execution



Troubleshooting section includes additional guidance

Sample Preparation

- Store FFPE tissue blocks at 4°C.

Sectioning Speed

- Sectioning speed is dependent and impacted by the desired thickness of the sections and the condition of the tissue. Harder and thicker sections require slow sectioning speed.
- Faster sectioning speed may lead to cracks or tears in the sections or damage to the tissue block.

Section Thickness

- Recommended section thickness is 5 μm .

Water Bath Temperature & Section Floating Time

- Optimal water bath temperature and section floating time are critical for tissue section expansion. 42°C is the recommended water bath temperature for most tissues. However, water bath temperature may need optimization based on the tissue type. Optimization should occur before utilization of a Xenium slide.
- Determine optimal water bath conditions before tissue placement on the Xenium slides by practicing section placement on a blank slide.
- If the tissue is taking too long to expand, turn the water bath temperature up by 1 or 2 degrees and let the section float for longer.

- If the tissue is expanding too quickly and dissociating, turn the water bath temperature down by 1 or 2 degrees and shorten the floating time.

Tissue Section Quality Control


- After section placement on blank slides, sections should be DAPI and hematoxylin and eosin (H&E) stained to examine tissue morphology.
- Use the H&E staining to look for signs of over or underfixation and sampling artifacts. Use this information to determine if scoring is needed to select the area of interest.

Xenium Slide Template

- Use the following diagram to verify that freshly placed tissue sections are compatible with the Xenium Slide. Reference the image below to draw the sample area on the back of blank slides.




Images are to scale if scaling settings are not modified (select "actual size" or "100%" to print to scale).

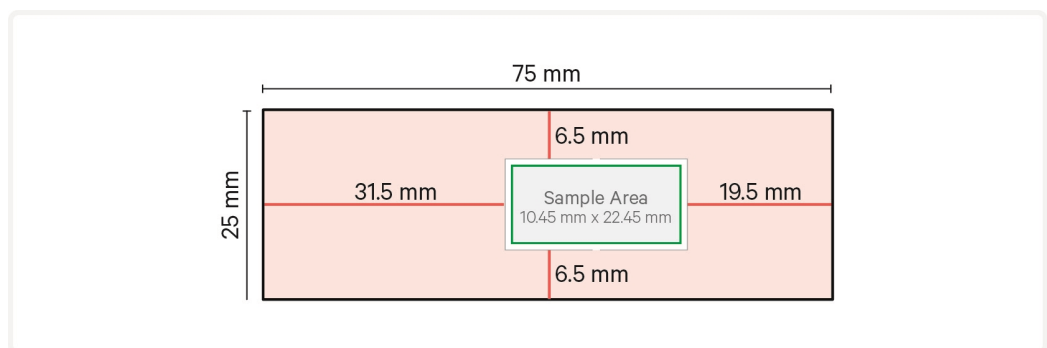

- Practice correct section placement within the representative frames using non-experimental blocks.


Section Placement on Xenium Slides

- Discard the first couple of sections after facing the block before placing sections on Xenium slides.
- Place the tissue section within the Sample Area on Xenium slides. Avoid covering the fiducials with tissue.

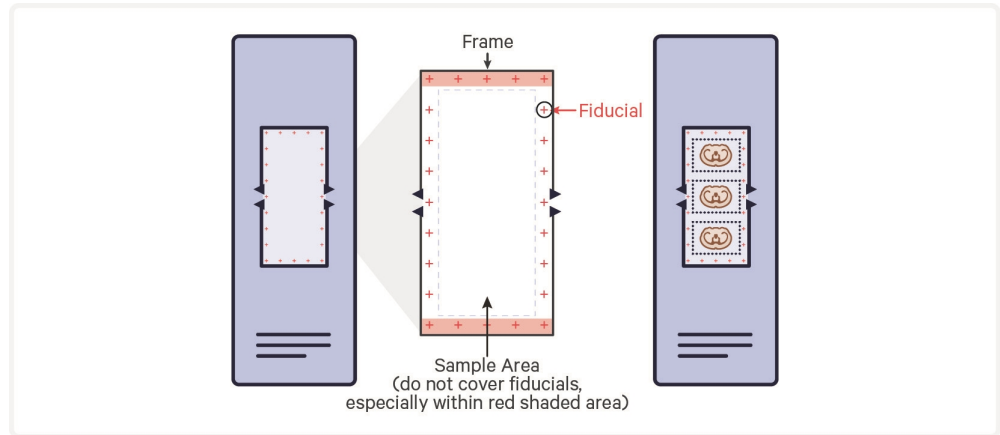

- To assist in section placement, trace the Sample Area on the back of the slide using the provided template in [Xenium Slide Template on the previous page](#).
- The section on the slides should be uniform without any cracks, tears, or folds.
- The wax surrounding each tissue section should not overlap other sections.

- Once sections are placed on Xenium slides, they cannot be repositioned as this would compromise slide integrity and assay performance.

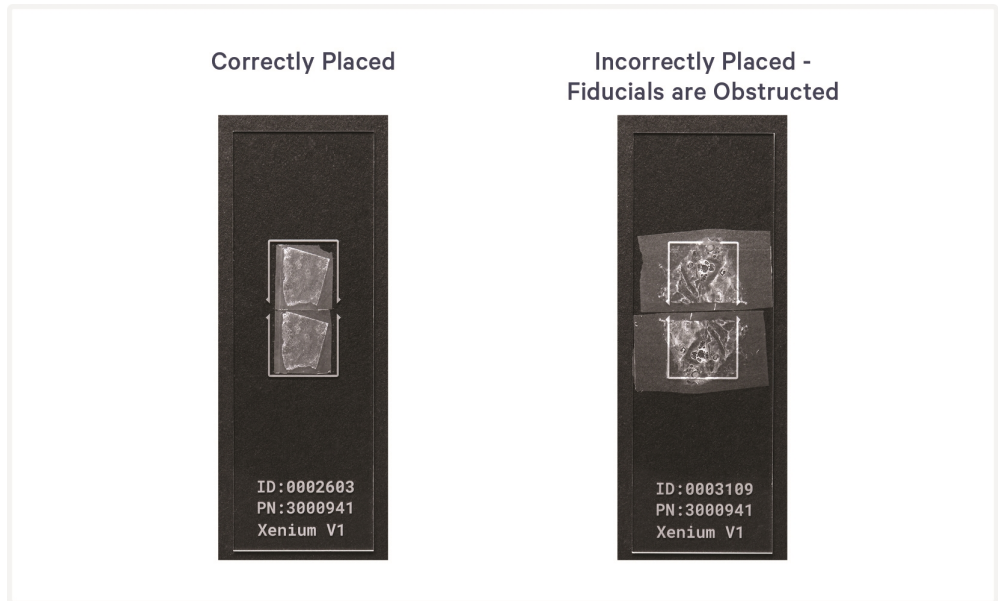

Optional Tissue Trimming & Scoring

FFPE tissue blocks can be trimmed or scored to fit multiple sections onto the Sample Area.

- **FFPE Tissue Block is smaller than Sample Area:** Paraffin around the embedded tissue in the FFPE tissue block should not be trimmed, and the section will fit the Sample Area.
- **FFPE Tissue Block is larger than Sample Area, but tissue is smaller than Sample Area:** Paraffin around the embedded tissue in the FFPE tissue block can be trimmed for the section to fit the Sample Area.
- **FFPE Tissue Block & Tissue are larger than Sample Area:** Paraffin around the embedded tissue in the FFPE tissue block can be trimmed, and the actual tissue can be scored to generate smaller sections to fit the Sample Area.
- Use a razor blade for trimming and scoring the tissue Block. See [Optional Trimming/Scoring the Block on page 59](#) for details.
- Alternatively, tissue sections may be sectioned and trimmed on a cutting mat. See [Alternative Trimming or Scoring of FFPE Block & Tissue on page 62](#) for details.
- Once the tissue has been trimmed and scored, use extra care during sectioning and section handling.

Tissue Detachment on Xenium Slides



- Monitor section adhesion on Xenium slides throughout the workflow.
- Tissue detachment during the workflow can negatively impact performance. If observed, contact support@10xgenomics.com.
- For more information, refer to Troubleshooting.

Handling Xenium Slides

Handling Xenium Slides Without Tissue Sections

- Store packaged slides at **-20°C**.
- DO NOT touch the surface of the slide.
- Prior to sectioning, slides should be equilibrated to room temperature for **30 min**.
- Once opened, the slide can remain at room temperature in a desiccator for up to one week.

Handling Xenium Slides Containing Tissue Sections

- Slides containing tissue sections that have been incubated at **42°C** for **3h** and dried overnight at room temperature in a desiccator can be stored for up to **4 weeks** at room temperature in a desiccator.

Xenium Slide Incubation

- After sectioning, slides with tissue sections must be dried with either a section dryer oven (preferred) or a thermocycler.

Incubation using a Section Dryer Oven


- a. Ensure slides have been dried with a fan at room temperature to remove water trapped on top of and under the section prior to using the dryer oven.
- b. Close the lid when incubating the slide in the oven.

Incubation on a Thermal Cycler

- a. Position a Xenium Thermocycler Adapter on a thermal cycler that is set at the incubation temperature.
 - Ensure that the Xenium Thermocycler Adapter is in contact with the thermal cycler surface uniformly.
- b. Place the slide on the Xenium Thermocycler Adapter with the tissue facing up.

- Ensure that the entire bottom surface of the slide is in contact with Xenium Thermocycler Adapter.

DO NOT close the thermal cycler lid when incubating the slide due to the risk of touching the tissue.

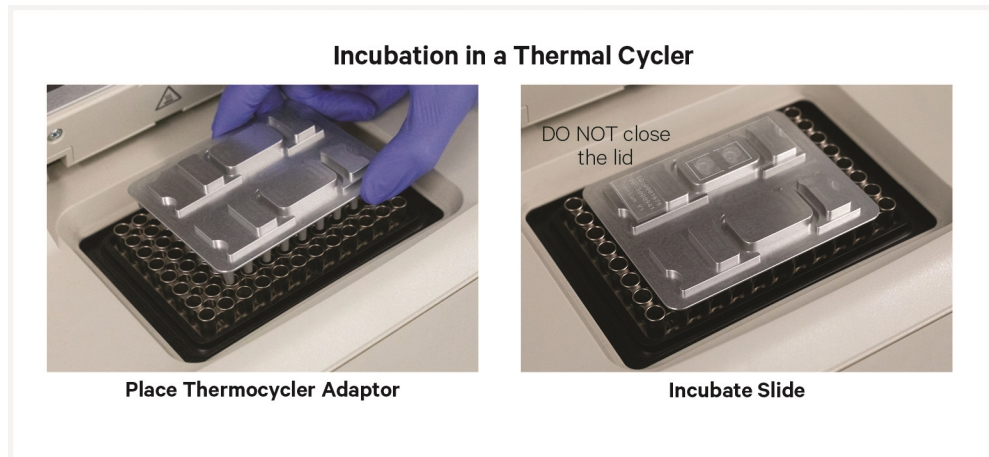


1. FFPE Tissue Sectioning, Section Placement, and Quality Assessment

Overview

This section provides guidance on choosing a quality assessment method, sectioning FFPE tissue blocks, section placement on blank slides using a water bath, and quality assessment. Ensure that tissue sections have been processed according to guidelines in [Tissue Handling, Fixation, and Embedding Guidelines](#) on page 12.



Xenium slides are not used for the quality assessment. Sectioning and placement on Xenium slides for the full workflow occur in [3.1 Section Placement on Xenium Slides](#) on page 41.

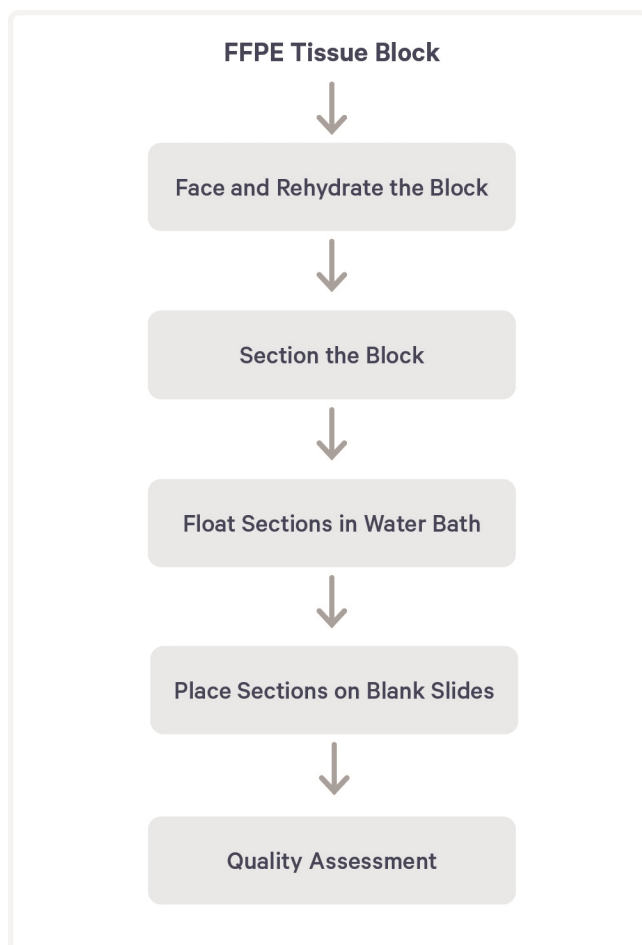

Choose a Quality Assessment Method

Choose one or more quality assessment methods from the following options. Though quality assessment is optional, 10x Genomics strongly recommends performing DAPI and H&E quality assessment on one or more serial sections prior to starting the Xenium assay. Quality assessment is performed after sections are placed onto blank slides.

DAPI Staining

DAPI is a nuclear stain that enables assessment of nuclei quality, a predictor of assay success. However, good nuclei quality is not an absolute determinant of assay success.

H&E Staining

H&E staining allows for observation of tissue damage and artifacts that may result from poor tissue handling, sectioning, or fixation. These artifacts are correlated with poor assay outcomes. However, identification of artifacts may require histology expertise. Additionally, blood in the H&E image may result in high autofluorescence. High autofluorescence does not necessarily correlate with poor assay outcomes.

DV200

DV200 assesses RNA integrity, where the DV200 score indicates the percentage of RNA fragments over 200 nucleotides in length. A DV200 score of less than 30% is correlated with low transcript density.

Face the Block and Rehydrate

FFPE tissue block is placed in a microtome and cut to face the tissue. The block is rehydrated in an ice bath.

Sectioning

The tissue block is sectioned using a microtome. A section may be saved at this step for optional DV200 assessment. See [DV200 Performance and Recommendations on page 34](#) for more information.

Section Placement

Sections are collected in a water bath and are allowed to float on the water surface until they are flat and free from wrinkles and folds. The optimal floating time depends upon the specific tissue type and should be empirically determined when working with new tissue types. Expanded tissue sections are placed on a blank slide for H&E staining.

Quality Assessment

Tissue sections on slides are deparaffinized prior DAPI and H&E staining. A deparaffinization protocol is provided in the Appendix. Perform DAPI staining according to any preferred protocol. A DAPI protocol is provided in the Appendix. After DAPI staining and imaging, perform H&E staining according to any preferred protocol. An H&E protocol is provided in the Appendix. DAPI and H&E may be performed on the same tissue section or on serial sections.

DV200 analysis: RNA is extracted from tissue sections and analyzed as described in [RNA Quality Assessment of FFPE Tissue Block on page 63](#).


1.0 Get Started

Items		10x PN	Preparation & Handling	Storage
Obtain				
<input type="checkbox"/>	Mounting Media	-	-	Ambient
<input type="checkbox"/>	Milli-Q Water	-	-	Ambient
<input type="checkbox"/>	Water Bath	-	Equilibrate to optimal temperature.	Ambient
<input type="checkbox"/>	Blank Slides	-		Ambient
<input type="checkbox"/>	Brushes	-		Ambient
<input type="checkbox"/>	Microtome	-		Ambient
<input type="checkbox"/>	Microtome blade	-		Ambient
<input type="checkbox"/>	Fan <i>(optional, but recommended)</i>	-		Ambient
<input type="checkbox"/>	Section Dryer Oven <i>(optional, but recommended)</i>	-	Equilibrate to desired temperature.	Ambient
<input type="checkbox"/>	Marker	-		Ambient
<input type="checkbox"/>	Coverslips	-		Ambient
<input type="checkbox"/>	Wide-bore pipettes	-		Ambient

1.1 Facing the Block

Before starting, wipe down all the surfaces and work areas with RNase Zap RNase decontaminating solution. If necessary, rewipe the area with 100% ethanol to quickly dry the surface.

- a. Remove tissue blocks from storage.
- b. Set the microtome to the 15 μm setting.
- c. Cut the tissue block at 15 μm until all of the edges of the tissue are exposed or until the region of interest is exposed. The block should be at **room temperature** during cutting.

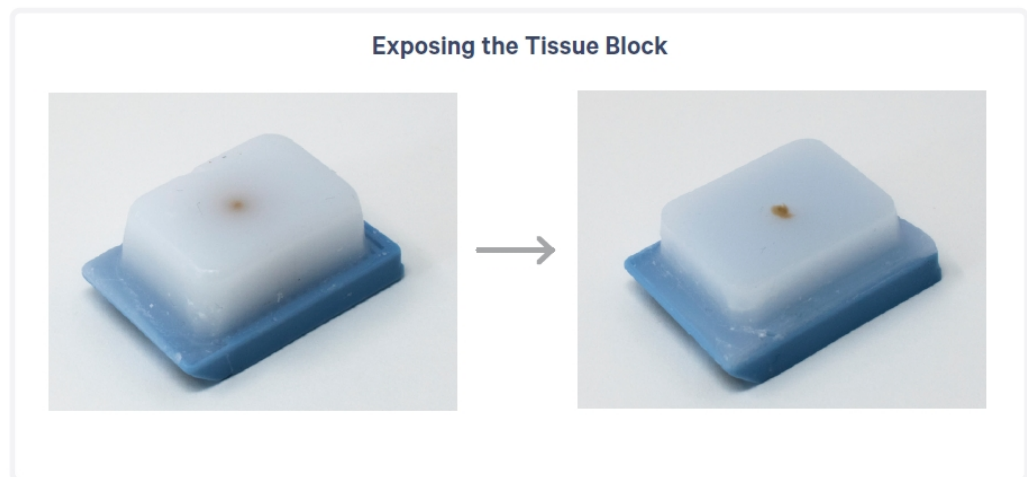


1.2 Sectioning

- a. Fill up a water bath with Milli-Q water and ensure that the temperature is set at **42°C** and free from bubbles & particulates by gliding a laboratory wipe over the water surface. Repeat this step between sectioning as and when necessary.



42°C is the recommended water bath temperature for most tissues. However, water bath temperature may need optimization based on the tissue type. Determine optimal water bath conditions before tissue placement on the Xenium slides by practicing section placement on a blank slide. See Tips & Best Practices for guidance on optimizing water bath temperature. To better visualize the tissue sections, a Lighted Tissue Floating Bath with LED illumination can be used instead of standard water bath.

Remove Bubbles



- b. Place blocks in the ice bath, ensuring that the tissue part is fully submerged. Ice should be from filtered water. If not available, freeze Milli-Q water ahead of tissue sectioning.
- c. Incubate on the ice bath for **10-30 min**. The incubation time depends upon the tissue type and the extent of dehydration. Extent of dehydration depends on processing method and age of tissue block.



Monitor the exposed tissue every 5-10 min during the ice bath incubation. The tissue surface should be smooth and shiny and free of bumps at the end of the incubation. Sectioning compression and shattering are usually due to insufficient hydration. For more information on tissue hydration, see Troubleshooting section.

FFPE Tissue Block in Ice Bath



- d.** Carefully wipe off the excess oils from a 35X Ultra disposable blade using a laboratory wipe with 100% ethanol. Let the ethanol evaporate before proceeding. Always use new blades for sectioning.
- e.** Secure the blade in the disposable blade holder of the microtome and place the knife guard over the blade to minimize injury. Ensure that the clearance angle is set to 10°. Set the microtome to 5 μm (or desired cutting thickness) for sectioning.
- f.** After hydration is complete, place the tissue block in the specimen clamp and align it with the blade. For tissue blocks with exposed tissue, discard the first few sections and start collection on subsequent sections.
- g.** To collect sections, place the paintbrush tip slightly above and parallel to the blade. Lift section by lightly touching the edge with the paintbrush while rotating the wheel handle.
- h.** With the help of the brush, pick section up. Immediately place it on the water surface of the water bath, making sure that the brush tip goes underneath and away from the section.
- i.** Proceed directly to Section Placement.


1.3 Section Placement on Blank Slides

- a. Allow sections to float for previously determined optimal time.
- b. Insert the slide into the water.
- c. Using the paintbrush or the probe, maneuver the section to the slide.

If sections float away from the slide, the slide can also be dipped into the water bath before section placement.

- d. Pull the slide up and out of the water, ensuring there are no air bubbles trapped underneath and set aside.

If sections require repositioning and the sections have not dried onto the slide, repeat section placement by resubmerging the slide and refloating sections in the water bath. Ensure that minimal water is trapped beneath the section and that the section does not disintegrate from extended floating in the water bath.

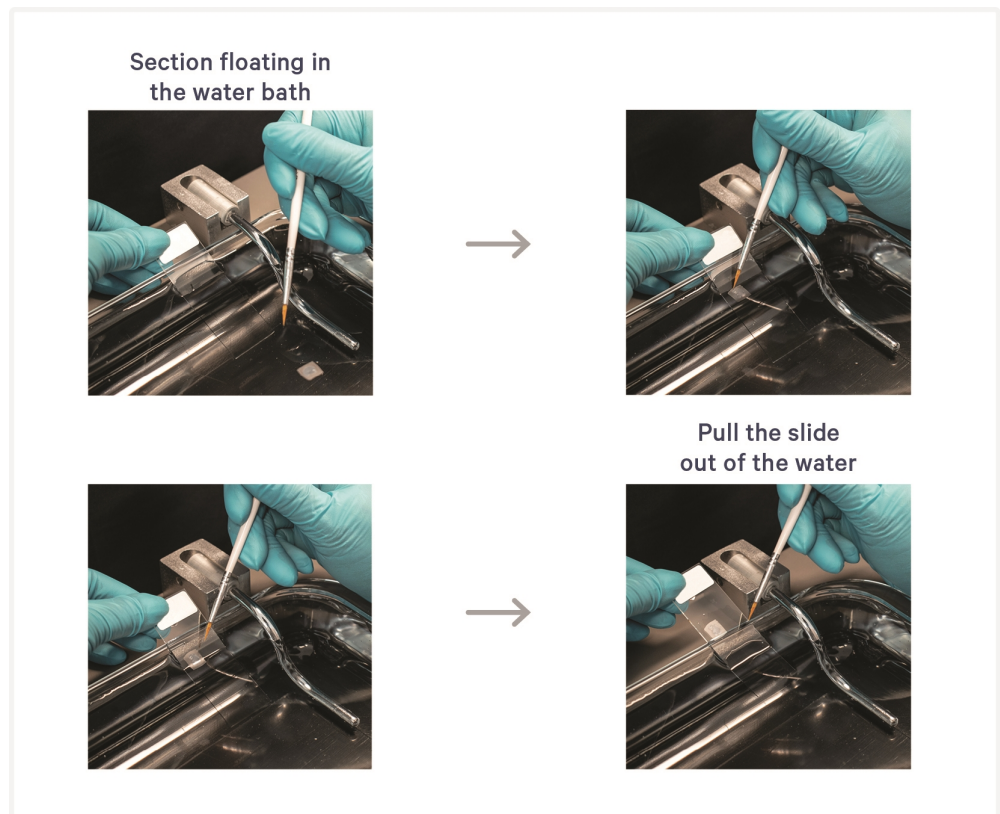

- e. Repeat, if needed, for additional sections, ensuring that the previous sections do not get re-submerged in the water.

- f. Dry tissue sections upright in a drying rack at room temperature until tissue is opaque and no water remains on top of or under the section. A fan may be used to assist in drying.



- g. Place the slides in a slide drying rack and incubate for **10 min** at **42°C** in an oven or thermal cycler.



See Tips & Best Practices for guidance on [slide incubation](#).



- h. Proceed to Deparaffinization & Quality Assessment.

1.4 Deparaffinization & Quality Assessment

Tissue sections on slides must be deparaffinized prior to quality assessment. A deparaffinization protocol is provided in the Appendix.


Quality assessment is composed of two parts: DAPI staining and H&E staining. Perform DAPI staining according to any preferred protocol. A DAPI protocol is provided in the Appendix. After DAPI staining and imaging, perform H&E staining according to any preferred protocol. An H&E protocol is provided in the Appendix. DAPI and H&E may be performed on the same tissue section or on serial sections.

1.5 DAPI Quality Assessment

Review the DAPI image under the microscope at 20x magnification. Examine several sections within a single DAPI-stained section to ensure assessment is comprehensive. Tissue sections suitable for the Xenium assay should have:

- Punctate nuclei that are clearly defined
- DAPI staining that does not appear washed out

Sections with poor DAPI staining are unlikely to generate good data. All samples in the images below were imaged under the same conditions (405 nm channel). After evaluating DAPI staining, proceed to [3. FFPE Tissue Sectioning & Section Placement on page 38](#) for placement of tissue sections on Xenium slides or proceed with additional quality assessment methods.

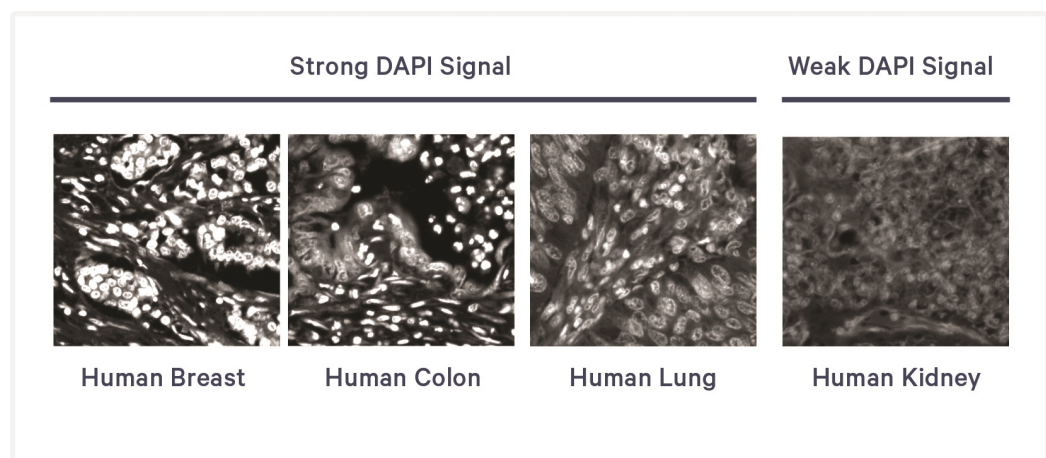


1.6 H&E Tissue Quality Assessment

Review the H&E image thoroughly to assess tissue quality and select area(s) of interest. If scoring the block or section is necessary, refer to [Optional Trimming/Scoring the Block on page 59](#).

Ensure that the tissue section is free from tissue processing and sectioning artifacts as shown in [Troubleshooting on page 43](#). Tissue processing artifacts may include improper fixation, squeeze/crush artifacts, and hemorrhaging. Examples are shown in the images below. If H&E staining was performed on the same tissue section used for DAPI quality assessment (see previous section), ensure that DAPI staining overlaps well with nuclei seen during H&E imaging.

If imaging reveals satisfactory tissue morphology, proceed with [2. Optional - Practice FFPE Tissue Sectioning & Section Placement on page 36](#) if additional sectioning practice is needed, [3. FFPE Tissue Sectioning & Section Placement on page 38](#) for placement of tissue sections on Xenium slides, or any additional quality assessment methods.

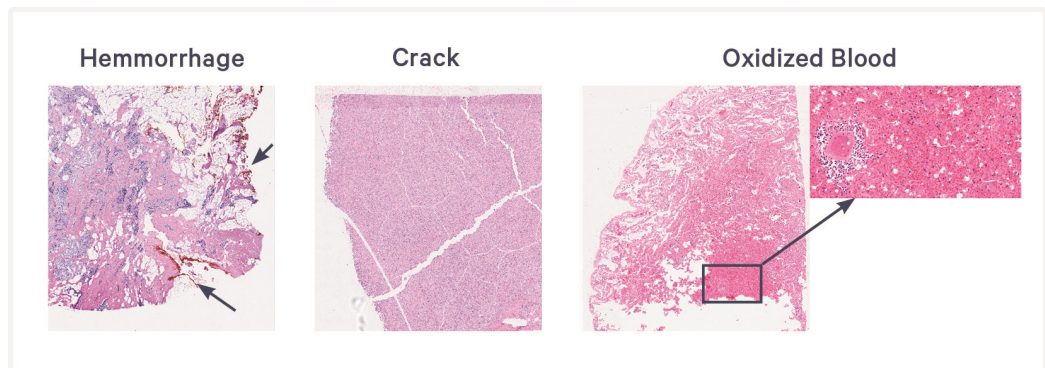

DV200 Performance and Recommendations

Assess DV200 according to preferred method. A DV200 method is provided in the Appendix. DV200 is a broad measurement of RNA quality and is influenced by factors including:

- Tissue block age, type and composition
- Region selected for RNA extraction
- Presence of diseased or necrotic regions
- Depth of section


- Fixation method
- Miscellaneous upstream tissue handling and processing

10x Genomics recommends that the tissues used in the Xenium In Situ assay should have a DV200 of >30%.

2. Optional - Practice FFPE Tissue Sectioning & Section Placement

Overview

This section provides guidance on sectioning FFPE tissue blocks and section placement on blank slides using a water bath. This practice step is optional. After examining the H&E tissue section, if necessary, score of the block to isolate the region of interest.

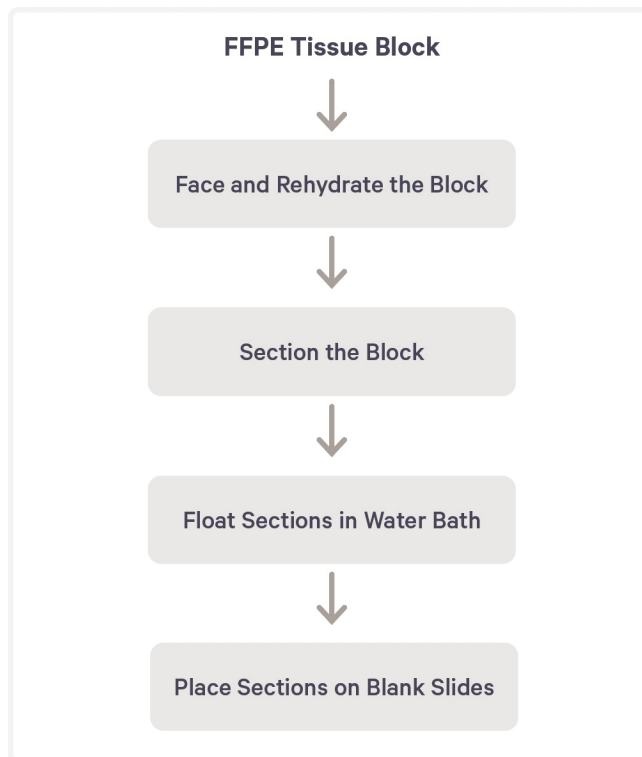

Face the Block and Rehydrate

FFPE tissue block is placed in a microtome and cut to face the tissue. Facing is only necessary for new, unused blocks. For tissue blocks with exposed tissue, discard the first few sections and start collection on subsequent sections. The block is rehydrated in an ice bath. Perform as described in step 1.

Sectioning

The tissue block is sectioned using a microtome to generate appropriately sized sections for blank slides. Perform as described in step 1.

Section Placement

Draw the template shown in [Xenium Slide Template on page 18](#) onto a blank slide to simulate the Sample Area on the Xenium slide. Sections are collected in a water bath and are allowed to float on the water surface until they are flat and free from wrinkles and folds. The optimal floating time depends upon the specific tissue type and should be empirically determined when working with new tissue types.


2.0 Get Started

Items	10x PN	Preparation & Handling	Storage
Obtain			
<input type="checkbox"/>	Milli-Q Water	-	Ambient
<input type="checkbox"/>	Water Bath	Equilibrate to optimal temperature.	Ambient
<input type="checkbox"/>	Blank Slides	-	Ambient
<input type="checkbox"/>	Brushes	-	Ambient
<input type="checkbox"/>	Microtome	-	Ambient
<input type="checkbox"/>	Microtome blade	-	Ambient
<input type="checkbox"/>	Fan <i>(optional, but recommended)</i>	-	Ambient
<input type="checkbox"/>	Section Dryer Oven <i>(optional, but recommended)</i>	Equilibrate to desired temperature.	Ambient
<input type="checkbox"/>	Marker	-	Ambient
<input type="checkbox"/>	Coverslips	-	Ambient

3. FFPE Tissue Sectioning & Section Placement

Overview

This section provides guidance on sectioning FFPE tissue blocks and section placement on the Xenium slides using a water bath.

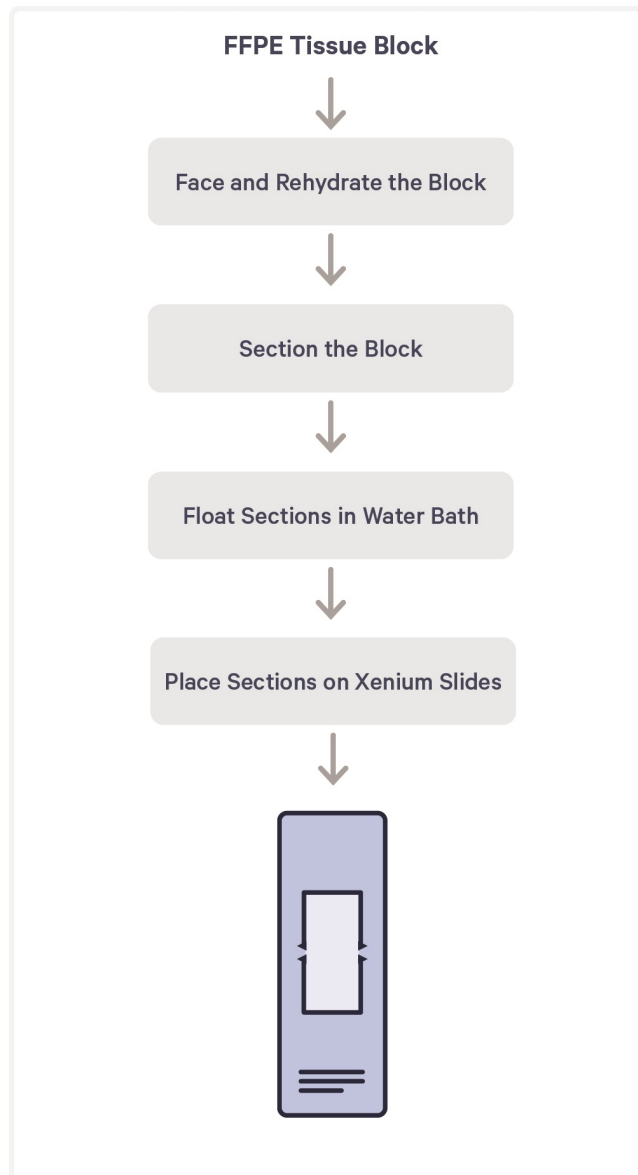

Face the Block and Rehydrate

FFPE tissue block is placed in a microtome and cut to face the tissue. Facing is only necessary for new, unused blocks. For tissue blocks with exposed tissue, discard the first few sections and start collection on subsequent

sections. The block is rehydrated in an ice bath. Perform as described in step 1.


Sectioning

The tissue block with exposed tissue is optionally trimmed or scored to make it compatible in size to the Sample Area on Xenium slides. The tissue block is then sectioned by a microtome to generate appropriately sized sections for Xenium slides. Perform as described in step 1.

Section Placement

Sections are collected in a water bath and are allowed to float on the water surface until they are flat and free from wrinkles and folds. The optimal floating time depends upon the specific tissue type and should be empirically determined when working with new tissue types. Expanded tissue sections are placed on the slide of choice. Prior to placing tissue sections on a Xenium slide, practice section placement on a blank slide. Do not obstruct the fiducials while placing tissue.

Slides are assembled into the Xenium Cassette with the etched label oriented towards the bottom. If holding the Xenium slide by the etched label for section placement, the slide will be rotated during cassette assembly and placement on the Xenium Analyzer. This results in an image that is rotated compared to initial section placement (refer to image below).

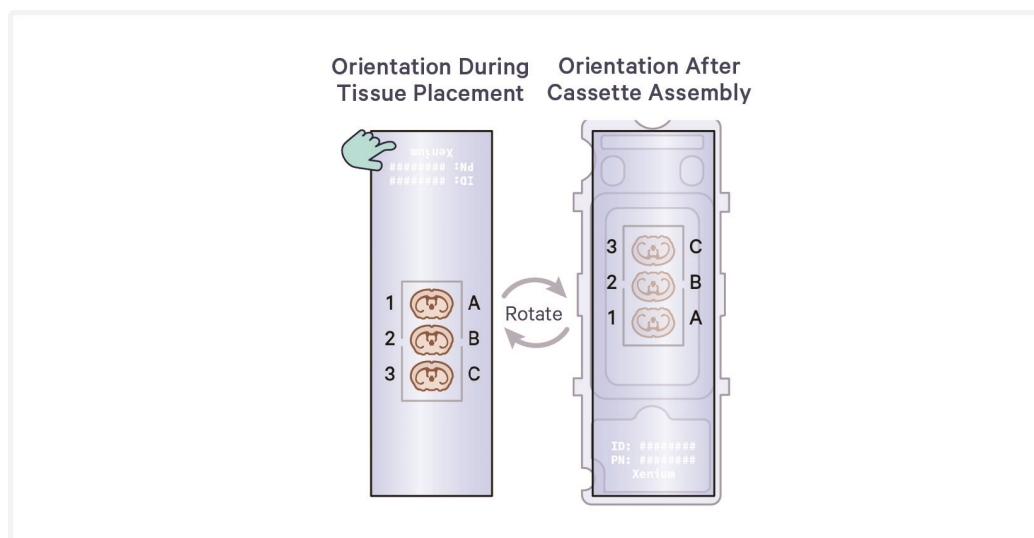

3.0 Get Started

Items	10x PN	Preparation & Handling	Storage
Equilibrate to room temperature			
<input type="checkbox"/>	Xenium Slides 3000941	Equilibrate at room temperature for 30 min prior to sectioning.	-20°C
Obtain			
<input type="checkbox"/>	Water Bath	-	Equilibrate to optimal temperature. Ambient
<input type="checkbox"/>	Brushes	-	Ambient
<input type="checkbox"/>	Microtome	-	Ambient
<input type="checkbox"/>	Microtome blade	-	Ambient
<input type="checkbox"/>	Fan <i>(optional, but recommended)</i>	-	Ambient
<input type="checkbox"/>	Section Dryer Oven <i>(optional, but recommended)</i>	-	Equilibrate to desired temperature. Ambient
<input type="checkbox"/>	Marker	-	Ambient

3.1 Section Placement on Xenium Slides

Optional: Before placing sections on Xenium slides, trace the Sample Area onto the back of the slide with a marker. Using an unsupported marker may compromise assay performance. See [Xenium Slide Template on page 18](#) for slide layout.

Prior to section placement, face, rehydrate, and section the block as described in step 1.

- a. Allow sections to float for previously determined optimal time.
- b. Insert the slide into the water.
- c. Using the paintbrush or the probe, maneuver the section to the top of the Sample Area on the slide.


If sections float away from the slide, Xenium slide can also be dipped into the water bath before section placement.

- d. Pull the slide up and out of the water, ensuring there are no air bubbles trapped underneath and set aside. Avoid covering the fiducial frame.

If sections require repositioning and the sections have not dried onto the slide, it may be possible to repeat section placement by resubmerging the slide and refloating sections in the water bath. Ensure that minimal water is trapped beneath the section and that the section does not disintegrate from extended floating in the water bath.



If sections are placed incorrectly, contact support@10xgenomics.com to troubleshoot.

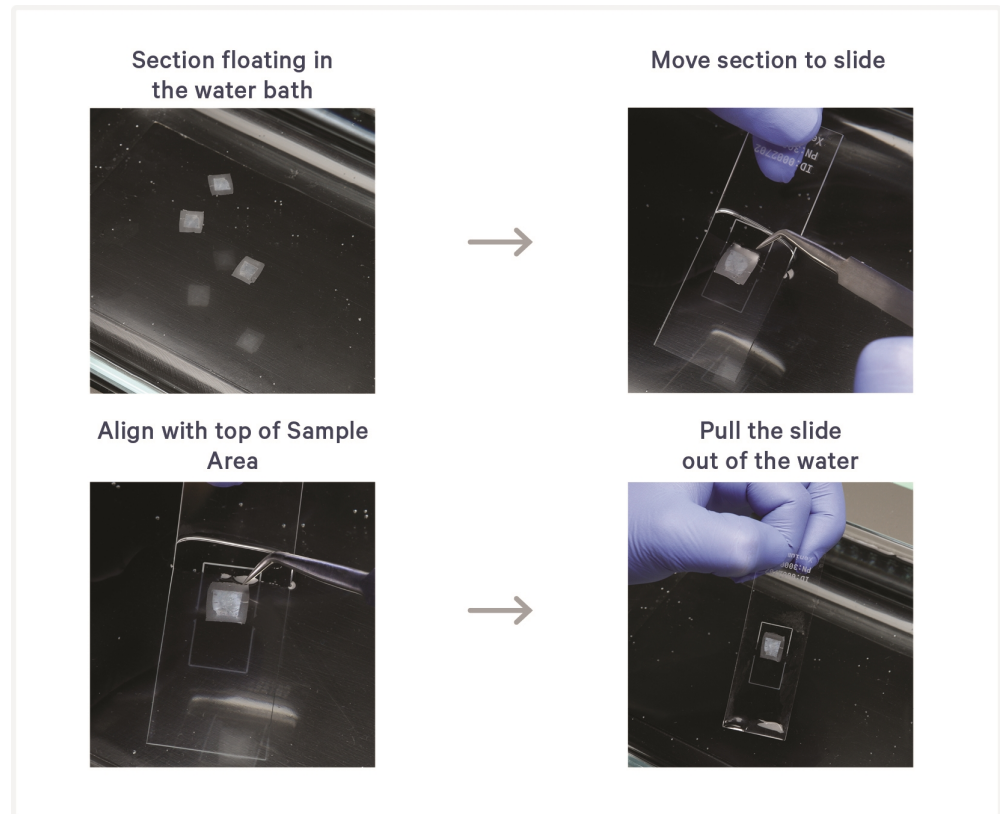

- e. Repeat for the remaining sections, ensuring that the previous sections do not get re-submerged in the water.
- f. Dry tissue sections upright in a drying rack at room temperature until tissue is opaque and no water remains on top of or under the section. A fan may be used to assist in drying. If no fan is used, slides may require extended drying time for up to **30 min** at **room temperature** to ensure no water remains under the section or until dry (inspect visually, do not touch tissue).
- g. Place the slides in a slide drying rack and incubate for **3 h** at **42°C** in an oven or thermal cycler.




See *Tips & Best Practices* for guidance on [slide incubation](#).

- h. *Optional, but recommended* - Place slides in a desiccator and keep overnight at **room temperature** to ensure proper drying. A lack of proper drying may result in tissue detachment or artifacts.
- i. After drying, proceed to deparaffinization and decrosslinking protocol (see References) or store the slide containing dry tissue sections at room temperature in a desiccator for up to **4 weeks**.




Troubleshooting

Ideal Floating Time Determination

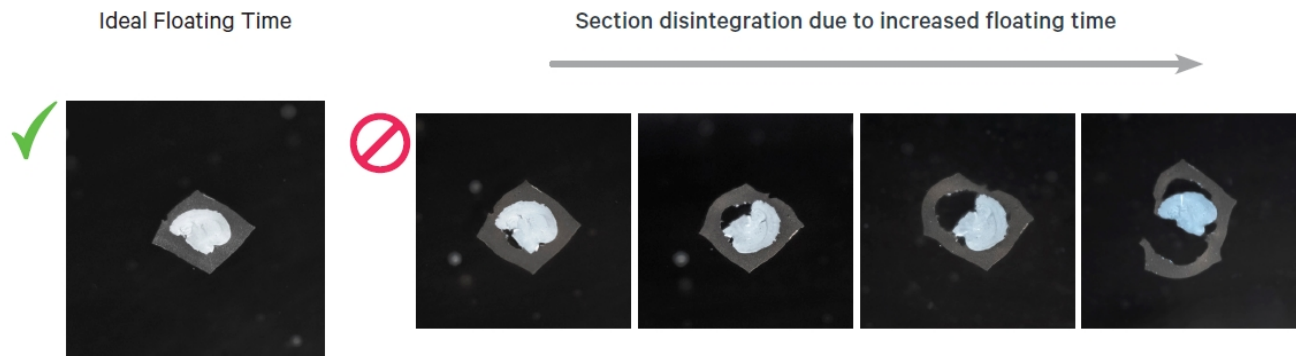

Common Issues when Processing FFPE Tissue Blocks


Section Phenotype	Tissue Characteristic	Guidance
Tissue is very dry	High Connective Tissue or High Cell Density Tissue	Soak block for an extended period of time. Re-soak tissue block every few sections.
Shattering, rapid expansion	High Adipose Tissue	If tissue is shattering, ensure tissue block is very cold by soaking the block in ice water for 10 min, re-soaking every few sections. If tissue expansion is occurring, lower water bath temperature to 37-39°C.
Rapid expansion	Low Cell Density Tissue	Lower water bath temperature to 37-39°C.

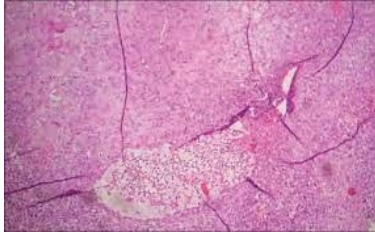Common Artifacts that cause Detachment or Misleading Data**Wrinkles****Causes**

- Section compression (due to warm block or dull blade) during sectioning leads to wrinkle formation. These wrinkles become permanent when placed in the water bath.
- Accumulated wax or static electricity on microtome parts also contribute to section compression.

Troubleshooting


- Ensure that the block is well hydrated.
- Adjust temperature down and increase float time.
- Gently and gradually lay FFPE sections onto water bath surface, lengthwise.
- Utilize a new blade.
- Ensure microtome is cleaned with 100% ethanol to minimize static and section compression (bunching on blade).

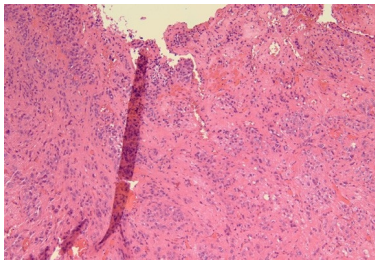Folds**Causes**

- Mostly happens when placing the section on the water bath especially when the section is uneven.
- If the fold is at the edge this most likely can happen during sectioning or mounting on the slide.

Troubleshooting


- Gently and gradually lay FFPE ribbons or sections onto water bath surface, lengthwise.
- If sections curl during sectioning, gently flatten them with a brush before floating.

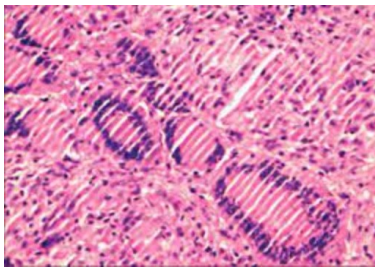Venetian Blinds or Shatter**Causes**

- Parallel lines in the section mostly appear due to dry tissue because of under-hydration of the block in the ice bath.
- Less likely due to dull blade or loose parts of the microtome.

Troubleshooting

- Increase incubation time of the block in ice bath.
- Tighten down components of microtome and make sure the blade is at a correct angle.

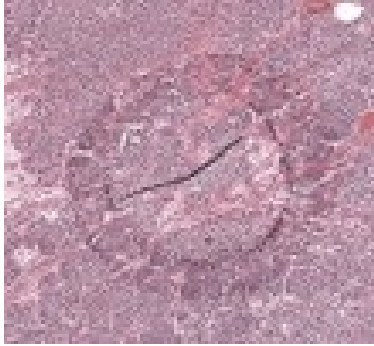Common Artifacts that cause Detachment or Misleading Spatial Data**Air Bubbles****Causes**

- Air bubbles from the bottom of the water bath can rise and stick under the section.

Troubleshooting

- Using a brush, gently remove the bubbles from the bottom of the water bath before floating the sections.

Waves


May be block-specific and easily observed under the microscope right after the section is picked up from the water bath. Minor waves can disappear after longer flotation in the water bath. Larger waves can create wrinkles or folds that are permanent after drying of the section.

Causes

- Tissue incompletely infiltrated with wax absorbs water faster during hydration step. When sections from such blocks are floated, the parts that absorbed enough water will have difficulty flattening and become wavy.

Troubleshooting

- Chill the block on a cold block or on ice avoiding contact with water.
- Submerge the block for 5-15 min in the ice bath for gentle hydration.
- Increase flotation times and/or temperature of the water bath.

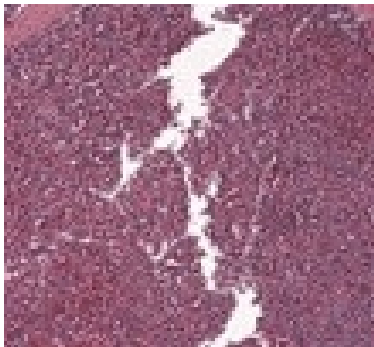Cracks**Causes**

- Dry and over-processed tissue can crack during sectioning.
- The cracks that are created before tissue embedding will be filled with wax when section is observed under the microscope after sectioning and wax will be washed away after deparaffinization or H&E staining.

Troubleshooting

- Prolonged hydration on the ice bath will most likely reduce the cracks.
- There is no solution for cracks created before tissue was embedded in wax.

Common Artifacts that cause Detachment or Misleading Spatial Data**Sweating****Causes**

- Inadequate dehydration or under-processing of the tissue causes parts of the section to attract water and create this blistering effect. Such sections can disintegrate in the water bath.
- The blisters consist of:
 - Xylene or xylene substitutes if the cause is under-processing and insufficient removal of xylene or
 - Water droplets if the cause is inadequate dehydration.

Troubleshooting

- Be cautious about how long the block is kept in ice bath. Long incubation time in ice bath can impact section quality and thus should be avoided.
- Long flotation time in the water bath should be avoided.

Water Retention**Causes**

- Sections from tissues that are under-processed or excessively hydrated before sectioning may retain water under the section mounted on a slide.
- Water will accumulate under section and cause uneven drying ultimately leading to detachment.

Troubleshooting

- Gently flicking the slide will help to get rid of the water. This is one of the most overlooked cause of detachment.

Disintegrating/Exploding Section**Causes**

- Sections from tissues that are under-processed and not sufficiently infiltrated with wax can rapidly absorb water and explode or gradually disintegrate in the water bath.
- Tissues that are not sufficiently dehydrated can show similar phenotypes.
- Floating at high temperatures (42-50°C) can exacerbate the disintegration.

Troubleshooting

- Chilling of the block should be mostly performed on ice or cold block (30-60 min).
- Exposure to water in ice bath during chilling should be kept to a minimum (5-10 min).
- Flotation water bath temperature should be lowered to 38-40°C.

Appendix

Deparaffinization & Quality Assessment

Tissue slides should be deparaffinized before quality assessment (DAPI and H&E staining)

Deparaffinization Items	10x PN	Preparation & Handling	Storage
Obtain			
<input type="checkbox"/>	Xylene	-	Ambient
<input type="checkbox"/>	Ethanol	-	Prepare Ethanol dilutions using Nuclease-free water.
<input type="checkbox"/>	Nuclease-free Water	-	Ambient
<input type="checkbox"/>	Forceps	-	Ambient
<input type="checkbox"/>	Slide Rack	-	Ambient
<input type="checkbox"/>	Coplin jars/Staining dishes	-	Ambient

DAPI Staining Items	10x PN	Preparation & Handling	Storage
Obtain			
<input type="checkbox"/>	DAPI Solution	-	Prepare 5 mg/ml DAPI in PBS to generate DAPI solution.
<input type="checkbox"/>	10X PBS	-	Prepare 1X PBS using nuclease-free water.
<input type="checkbox"/>	Slide Mailer	-	Ambient
<input type="checkbox"/>	Glycerol Mounting Medium	-	The dilution below is not necessary if stock glycerol is already at 85%. Invert to mix. Briefly centrifuge to remove bubbles.

Glycerol Mounting Medium 1 slide = 1 Tissue Slide	Stock	Final	1 Slide (µl)	2 Slides +15% (µl)	4 Slides +15% (µl)
Glycerol	100%	85%	127.5	293.3	586.5
Nuclease-free Water	-	-	22.5	51.7	103.5
Total	-	-	150.0	345.0	690.0

H&E Staining Items	10x PN	Preparation & Handling	Storage	
Obtain				
<input type="checkbox"/>	Hematoxylin	-	-	Ambient
<input type="checkbox"/>	Eosin	-	-	Ambient
<input type="checkbox"/>	Bluing Reagent	-	-	Ambient
<input type="checkbox"/>	Mounting Media	-	-	Ambient
<input type="checkbox"/>	Xylene	-	-	Ambient
<input type="checkbox"/>	Ethanol	-	Prepare Ethanol dilutions using Milli-Q water.	Ambient
<input type="checkbox"/>	Forceps	-	-	Ambient
<input type="checkbox"/>	Coplin Jars/Staining Dishes	-	-	Ambient
<input type="checkbox"/>	Milli-Q Water	-	-	Ambient

For Deparaffinization:

Prepare all buffers fresh according to the tables below.

- a. Prepare eight total coplin jars for deparaffinization steps. Prepare Ethanol dilutions using Nuclease-free water.

For Deparaffinization		
Items	Preparation & Handling	
<input type="checkbox"/> Xylene	Label two coplin jars as Xylene Jar 1 and 2. Fill to capacity with xylene in each.	
<input type="checkbox"/> 100% Ethanol	Label two coplin jars as 100% Ethanol Jar 1 and 2. Fill to capacity with 100% ethanol.	
<input type="checkbox"/> 96% Ethanol	Label two coplin jars as 96% Ethanol Jar 1 and 2. Fill to capacity with 96% ethanol.	
<input type="checkbox"/> 70% Ethanol	Label one coplin jar as 70% Ethanol Jar. Fill to capacity with 70% ethanol.	
<input type="checkbox"/> Nuclease-free water	Label one coplin jar as Nuclease-free Water Jar. Fill to capacity with Nuclease-free water.	



Alternatively, a slide staining dish can be used in place of a coplin jar. Adjust volumes accordingly. Use xylene-resistant dishes, gloves, and forceps during workflow. Prepare fresh reagents after every 20 slides or every week (whichever comes first).

Deparaffinization

Deparaffinization steps should be performed in a fume hood due to the hazardous nature of xylene. Xylene jars should be covered at all times to prevent evaporation.




The instructions apply to both Xenium v1 and Xenium Prime assays. The consumables are referred to generically without always citing the version suffix. Based on the assay choice, always ensure that either Xenium v1 or Xenium Prime specific reagents and consumables are used.

- a. Retrieve the slide with tissue sections from the desiccator after overnight drying.


Remove any marker annotations on slide using a lint-free laboratory wipe and 100% Ethanol.

- b. Place slide in a Section Dryer Oven and incubate uncovered at **60°C** for **30 min**.


Keep the oven lid closed during incubation.

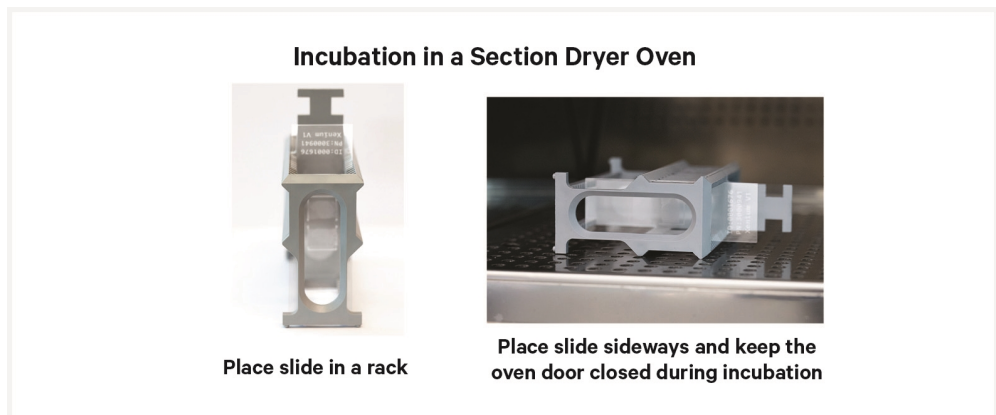

Alternatively, place a Thermocycler Adaptor on a thermal cycler set at **60°C**. Place slide on the Thermocycler Adaptor with the tissue side facing up and incubate at **60°C** for **30 min**. **DO NOT** close the thermal cycler lid.

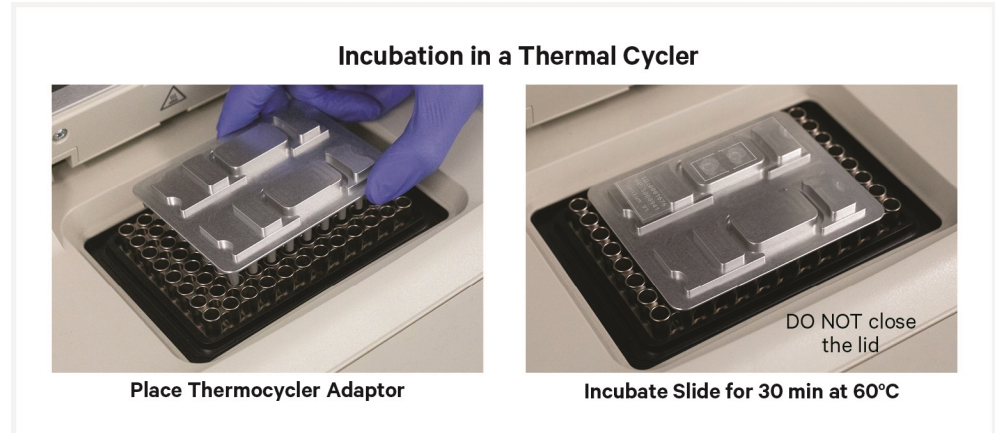

- c. Remove from the oven or thermal cycler and allow the slide to cool down to **room temperature** for **7 min.**
- d. Gently immerse slide in the Xylene Jar 1. Secure the jar cap to prevent xylene loss.

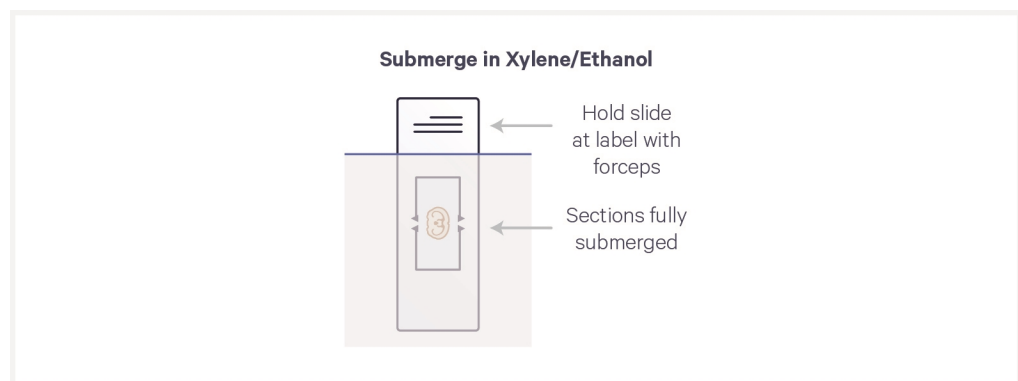

Hold slide at label with forceps for xylene immersion steps. When immersing slides in xylene, ensure that the tissue sections are completely submerged.

- e. Incubate for **10 min.**
- f. Gently immerse slide in the Xylene Jar 2 and incubate for **10 min.**
- g. Gently immerse slide in the 100% Ethanol Jar 1 for **3 min.**

Hold slide at label with forceps for ethanol immersion steps. When immersing slides in ethanol, ensure that the tissue sections are completely submerged.

- h. Gently immerse slide in the 100% Ethanol Jar 2 for **3 min.**
- i. Gently immerse slide in the 96% Ethanol Jar 1 for **3 min.**

- j.** Gently immerse slide in the 96% Ethanol Jar 2 for **3 min.**
- k.** Gently immerse slide in the 70% Ethanol Jar for **3 min.**
- l.** Gently immerse slide in the Nuclease-free water Jar for **20 sec.**

Proceed directly to DAPI staining. Leave slide in water until DAPI reagents have been prepared.

DAPI Staining


- a.** Place tissue slide on a flat, clean, nonabsorbent work surface.
- b.** Add **500 µl** DAPI solution per slide to uniformly cover all tissue sections.
- c.** Incubate **1 min** in the dark at **room temperature.**
- d.** Discard reagent by holding slides at an angle with the bottom edge in contact with a laboratory wipe
- e.** Add **1 ml** 1X PBS per slide to uniformly cover all tissue sections.
- f.** Incubate **1 min** in the dark at **room temperature.**
- g.** Discard reagent by holding slides at an angle with the bottom edge in contact with a laboratory wipe
- h.** Repeat steps e-g twice more for a total of three washes.
- i.** Wipe excess liquid from the front and back of the slides without touching the tissue section.

Coverslipping

Before mounting the coverslip, ensure that the slide is dry. Moisture on the surface of the slide may result in faulty mounting. Wipe away any residual droplets with a lint-free laboratory wipe.

- a.** Place slide on a flat, clean, non-absorbent work surface.
- b.** Using a **wide-bore** pipette tip, add **150-200 µl** Glycerol Mounting Medium to uniformly cover all tissue sections on the slide.
- c.** Apply the coverslip at an angle on one end of the slide. Slowly lower the coverslip, without introducing bubbles. Allow mounting media to spread and settle.
- d.** If needed, remove any large excess of mounting media by carefully wicking away from the edge of the coverslip with a lint-free laboratory wipe. Be careful not to move coverslip and disturb the tissue.

- e. Once coverslipping is complete, **immediately** proceed with imaging. See [1.5 DAPI Quality Assessment on page 33](#) for information on evaluating DAPI staining. Underexposure may result in inaccurate assessment of DAPI quality. Begin by overexposing samples, then reducing exposure until the resolution improves. If possible, process a control section in parallel from a block that has yielded good data.

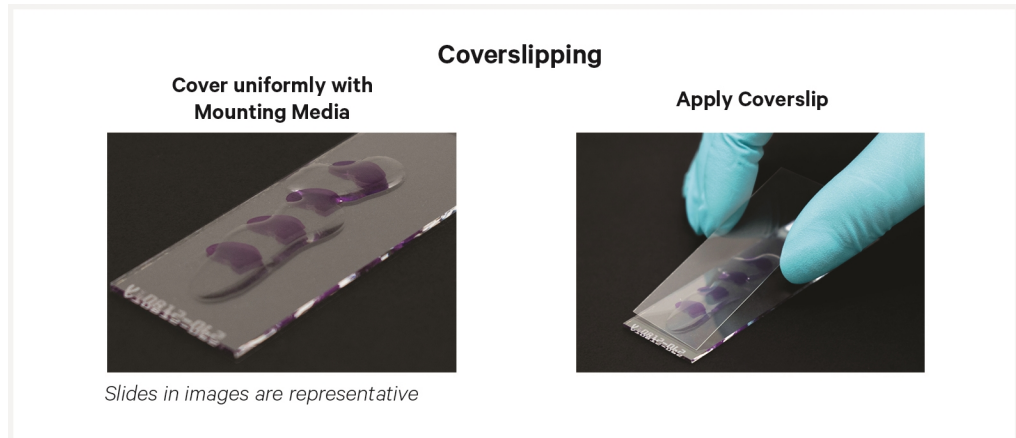


Coverslip Removal

- a. Dispense **800 ml** Milli-Q water in a beaker. Up to 10 slides may be processed using this beaker.
- b. Immerse slides sideways in the beaker containing **800 ml** water with the coverslipped surface fully sideways to prevent the coverslip from dragging across the tissue.
- c. Hold slides in water until the coverslip slowly separates away from the slide.



To avoid tissue section damage or detachment, DO NOT move the slide up and down, shake forcibly, or manually move the coverslip.

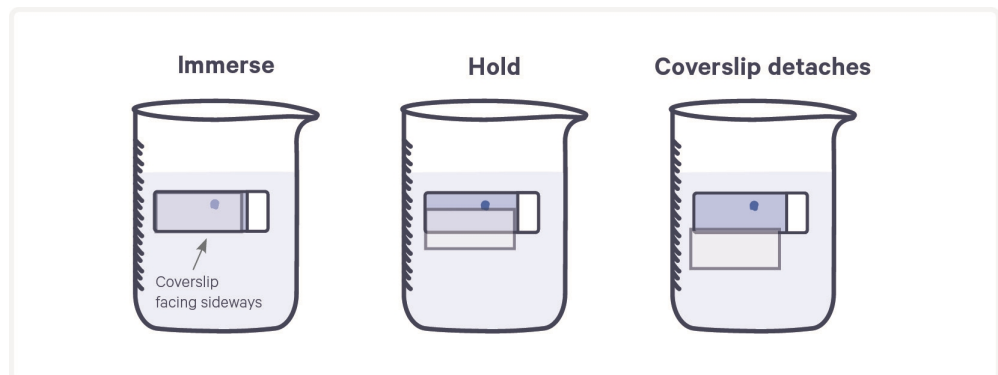

- d. Gently immerse slides 30x in water to ensure all Mounting Medium is removed.
- e. Wipe the back of the slide with a laboratory wipe. Place on a flat, clean, nonabsorbent work surface and air dry for **5 min**.
- f. Proceed with H&E Staining.

H&E Preparation



Prepare buffers in appropriate sized conical tube or bottle and transfer carefully to corresponding coplin jar.

- a. Filter Hematoxylin & Eosin solutions using filter paper before starting H&E Staining protocol.
- b. Prepare sixteen total coplin jars for H&E Staining steps.

For H&E Staining		
Items	Preparation & Handling	
<input type="checkbox"/> Hematoxylin Solution	Label one coplin jar as Hematoxylin Jar. Fill to capacity with Mayer's Hematoxylin Solution.	
<input type="checkbox"/> Bluing Solution	Label one coplin jar as Bluing Solution Jar. Fill to capacity with Bluing Solution.	
<input type="checkbox"/> 70% Ethanol	Label one coplin jar as 70% Ethanol Jar. Fill to capacity with 70% ethanol.	
<input type="checkbox"/> 95% Ethanol	Label three coplin jars as 95% Ethanol Jar 1, 2, and 3. Fill to capacity with 95% ethanol.	
<input type="checkbox"/> Eosin Solution	Label one coplin jar as Eosin Solution Jar. Fill to capacity with Eosin Solution.	
<input type="checkbox"/> 100% Ethanol	Label two coplin jars as 100% Ethanol Jar 1 and 2. Fill to capacity with 100% Ethanol.	
<input type="checkbox"/> Xylene	Label two coplin jars as Xylene Jar 1 and 2. Fill to capacity with Xylene.	
<input type="checkbox"/> Milli-Q Water	Label five coplin jars as Milli-Q Water Jar 1, 2, 3, 4, and 5. Fill to capacity with Milli-Q Water.	



Alternatively, a slide staining dish can be used in place of a coplin jar. Adjust volumes accordingly. Use xylene-resistant dishes, gloves, and forceps during workflow.

H&E Staining

H&E Staining steps should be performed in a fume hood due to the hazardous nature of xylene. Xylene jars should be covered at all times to prevent evaporation.

- a. Gently immerse slide in the Milli-Q Water Jar 1 for **2 min** at **room temperature**.



Water immersions may be performed in glass beakers containing Milli-Q water, if preferred.

- b. Gently immerse slide in the Hematoxylin Solution Jar for **20 min** at **room temperature**.



Substitution of Hematoxylin with a brand other than the recommended option may lead to tissue staining that is darker than anticipated following 20 min incubation.

- c. Gently immerse slide in the Milli-Q Water Jar 2 for **1 min** at **room temperature**.

- d. Gently immerse slide in the Milli-Q Water Jar 3 for **1 min** at **room temperature**.

- e. Gently immerse slide in the Milli-Q Water Jar 4 for **1 min** at **room temperature**.

- f. Gently immerse slide in the Bluing Solution Jar for **1 min** at **room temperature**.

- g. Gently immerse slide in the Milli-Q Water Jar 5 for **1 min** at **room temperature**.

- h. Gently immerse slide in the 70% Ethanol Jar for **3 min** at **room temperature**.

- i. Gently immerse slide in the 95% Ethanol Jar 1 for **3 min** at **room temperature**.

- j. Gently immerse slide in the Eosin Solution Jar for **2 min** at **room temperature**.

- k. Gently immerse slide in the 95% Ethanol Jar 2 for **30 sec** at **room temperature**.

- l. Gently immerse slide in the 95% Ethanol Jar 3 for **30 sec** at **room temperature**.

- m.** Gently immerse slide in the 100% Ethanol Jar 1 for **30 sec** at **room temperature**.
- n.** Gently immerse slide in the 100% Ethanol Jar 2 for **30 sec** at **room temperature**.
- o.** Gently immerse slide in the Xylene Jar 1 for **3 min** at **room temperature**.
- p.** Gently immerse slide in the Xylene Jar 2 for **3 min** at **room temperature**.

Coverslipping

Before mounting the coverslip, ensure that the slide is dry by gently flicking the slide to remove any droplets. Moisture on the surface of the slide may result in faulty mounting. Wipe away any residual droplets with a lint-free laboratory wipe.




The mounting medium used for mounting H&E-stained sections is different than what was used to mount slides after DAPI staining. Ensure that the appropriate mounting media is used.

- a. Place slide on a flat, clean, non-absorbent work surface.
- b. Using a **wide-bore** pipette tip, add **150-200 μ l** mounting media to uniformly cover all tissue sections on the slide.
- c. Apply the coverslip at an angle on one end of the slide. Slowly lower the coverslip, without introducing bubbles. Allow mounting media to spread and settle.
- d. If needed, remove any large excess of mounting media by carefully wicking away from the edge of the coverslip with a lint-free laboratory wipe. Be careful not to move coverslip and disturb the tissue.
- e. Dry the coverslipped slide for **30 min** at **room temperature**.
- f. Once coverslipping is complete, **immediately** proceed with imaging.



If imaging reveals satisfactory tissue morphology, proceed with [3. FFPE Tissue Sectioning & Section Placement on page 38](#).

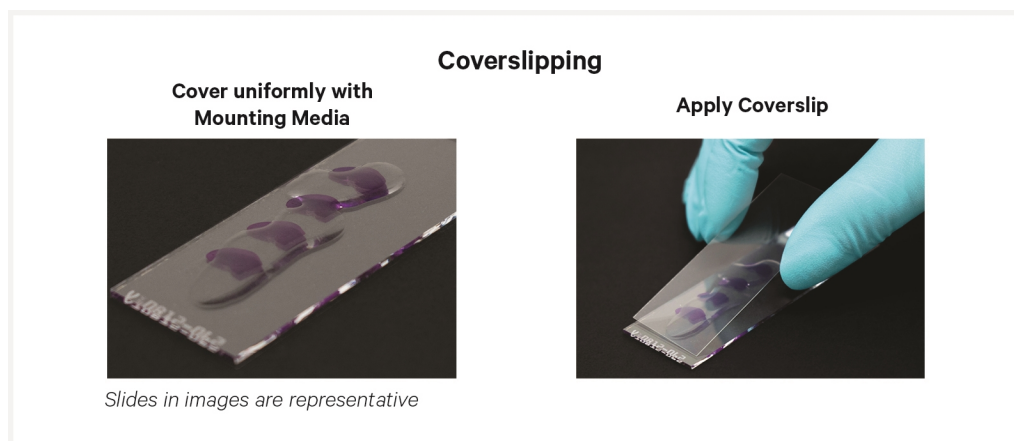

Optional Trimming/Scoring the Block


Before starting, wipe down all surfaces and work areas with RNaseZap RNase decontaminating solution. If necessary, rewipe the area with 100% ethanol to quickly dry the surface. Tissue sections placed on the Xenium slide should not obscure the fiducial frame. To ensure proper fit, the FFPE tissue block can be trimmed or scored as described below.

FFPE Tissue Block is larger than Sample Area, but tissue is smaller than Sample Area

For tissue samples that fit the Sample Area and are embedded in a large tissue block, the excess paraffin around the tissue can be trimmed to remove the excess and obtain smaller sections that fit the Sample Area.

- After facing, remove the tissue block from the microtome and start trimming.
- Using a razor blade, remove excess paraffin from around the tissue, so it is not larger than the Fiducial frame.
- Retain paraffin edges around the tissue samples to enhance tissue attachment on the slide.

Trimming large tissue block containing tissues that fit the Sample Area

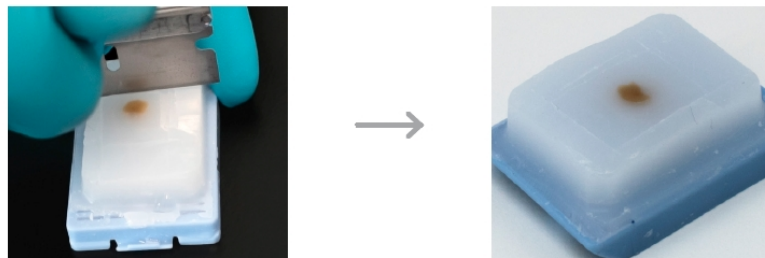


FFPE Tissue Block & Tissue are larger than Sample Area

Tissue samples larger than the Sample Area can be scored using a razor blade to generate smaller sections.

- Remove the tissue block from the microtome and start scoring.
- To score, lightly glide a razor blade over the surface of the tissue to introduce a shallow cut. This should yield approximately 10-15 trimmed


sections. A deep incision may lead to tissue damage and disintegration.

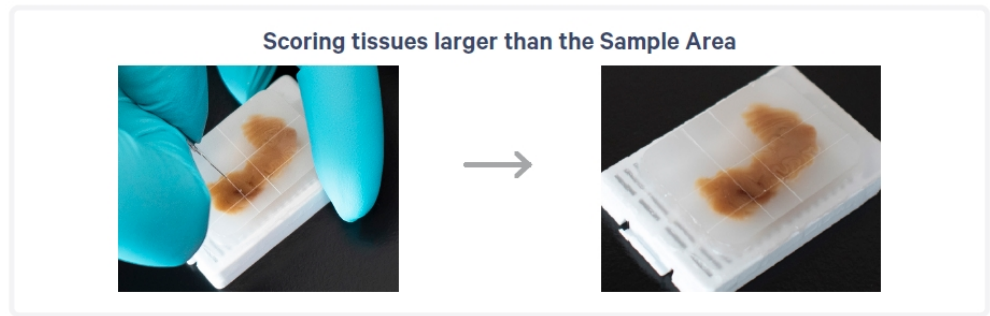

Scoring Configurations


Region of interest (ROI) is at the Top or Bottom of the Tissue

- If the ROI is at the bottom of the tissue, remove excess wax such that only three scoring cuts are necessary.
- This configuration may prevent curling of the ROI, as the excess wax at the top of the block may curl before affecting the ROI
- Retain paraffin edges around the tissue samples to enhance tissue attachment on the slide.

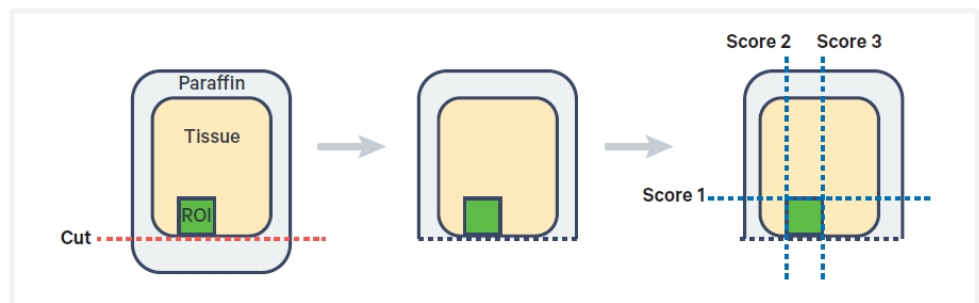

ROI is in the Middle of the Tissue

- If the ROI is in the middle of the tissue, make four scoring cuts as shown below.
- To prevent curling, place the brush over the edge of the ROI as the blade crosses the section. Avoid cutting the brush bristles on the blade.

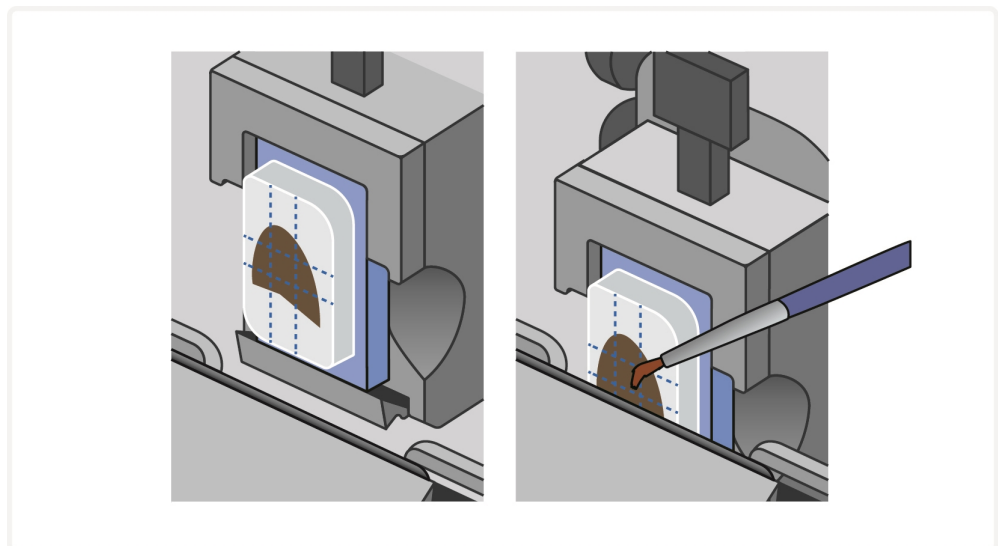


Alternative Trimming or Scoring of FFPE Block & Tissue



Keep all surface and materials RNase free. Avoid tearing of the FFPE sections during cutting. Keep the 5 µm FFPE sections from curling.


Set the microtome to 5 µm for tissue block and begin sectioning

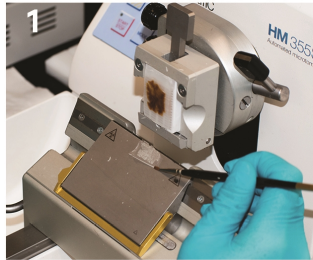

Collect sections with a paintbrush and place onto a cutting mat




Cut tissue sections into to fit in the Sample Area of the Xenium slide

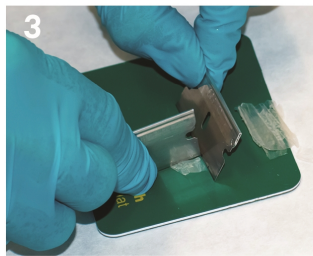


Place sections in the water bath



Align section with Sample Area

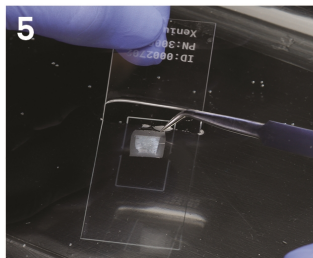

Pull the slide out of the water

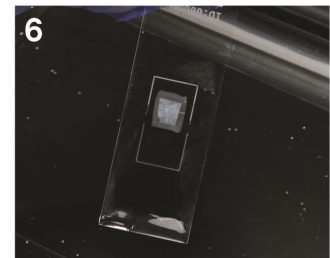

Shipping Guidance

- After sectioning, slides can be stored at **room temperature** in a desiccator.
- When ready for shipment, place up to 2 slides in a slide mailer with desiccant in a sealed bag.
- Ship in a styrofoam or cooler box with cool packs.

RNA Quality Assessment of FFPE Tissue Block

This section provides guidance on determining the RNA quality of the tissue block by calculating DV200 of RNA extracted from freshly collected tissue sections.

Mean RNA fragment size is a reliable determinant of RNA quality. This requires a measurement of the percentage of total RNA fragments >200 nucleotides (DV200) for RNA quality assessment upstream of library preparation. For more information on DV200, see [DV200 Performance and Recommendations on page 34](#).

Before starting RNA extraction, apply RNaseZap to a paper towel and wipe work surface, centrifuge rotor and shafts of the pipettes. Rinse with RNase-free water and then wipe dry. The electrodes of the Bioanalyzer can also be cleaned with RNaseZap by following Agilent decontamination procedure.

- a.** Collect 10 μm tissue sections for RNA extraction during FFPE block sectioning. Discard the first few sections if the block was already exposed. The required number of sections depends upon tissue size. Consult RNA extraction kit manufacturer instructions to determine the appropriate number of sections. See below for guidance:
 - Collect ~4 sections for smaller tissues ($\leq 6.5 \times 6.5 \text{ mm}$)
 - Collect 1-2 sections for larger tissues ($\geq 6.5 \times 6.5 \text{ mm}$)
- b.** Place the sections inside a **pre-cooled**, RNase-free microcentrifuge tube. Sections may be stored at **-80°C** for **long-term** storage. For sections stored at **-80°C**, equilibrate to **room temperature** for **5 min** before adding the deparaffinization solution.
- c.** Proceed to RNA extraction using RNeasy FFPE Kit and follow manufacturer's instructions.
- d.** Using a Nanodrop or Qubit Fluorometer, measure RNA concentration to determine the appropriate dilution for DV200 evaluation using the RNA

6000 Pico Kit or TapeStation High Sensitivity Kit. RNA outside of the recommended concentration may lead to inaccurate DV200 evaluation.

- e. Store purified RNA at **-80°C** for **long-term** storage or immediately proceed to DV200 evaluation using either the Agilent RNA 6000 Pico Kit or TapeStation High Sensitivity Kit. Follow manufacturer's instructions (Agilent) for DV200 evaluation.

References

1. Xenium In Situ for FFPE – Deparaffinization & Decrosslinking Demonstrated Protocol (CG000580)

Document Revision Summary

Document Number	CG000578
Title	Xenium In Situ for FFPE – Tissue Preparation Guide
Revision	Rev D
Revision Date	June 2024
Specific Changes	<ul style="list-style-type: none">• Added tissue handling, fixation, and embedding guidance• Added DAPI quality assessment guidance

© 2024 10x Genomics, Inc. (10x Genomics). All rights reserved. Duplication and/or reproduction of all or any portion of this document without the express written consent of 10x Genomics, is strictly forbidden. Nothing contained herein shall constitute any warranty, express or implied, as to the performance of any products described herein. Any and all warranties applicable to any products are set forth in the applicable terms and conditions of sale accompanying the purchase of such product. 10x Genomics provides no warranty and hereby disclaims any and all warranties as to the use of any third-party products or protocols described herein. The use of products described herein is subject to certain restrictions as set forth in the applicable terms and conditions of sale accompanying the purchase of such product. A non-exhaustive list of 10x Genomics' marks, many of which are registered in the United States and other countries can be viewed at: www.10xgenomics.com/trademarks. 10x Genomics may refer to the products or services offered by other companies by their brand name or company name solely for clarity, and does not claim any rights in those third-party marks or names. 10x Genomics products may be covered by one or more of the patents as indicated at: www.10xgenomics.com/patents. The use of products described herein is subject to 10x Genomics Terms and Conditions of Sale, available at www.10xgenomics.com/legal-notices, or such other terms that have been agreed to in writing between 10x Genomics and user. All products and services described herein are intended FOR RESEARCH USE ONLY and NOT FOR USE IN DIAGNOSTIC PROCEDURES.

The use of 10x Genomics products in practicing the methods set forth herein has not been validated by 10x Genomics, and such non-validated use is NOT COVERED BY 10X GENOMICS STANDARD WARRANTY, AND 10X GENOMICS HEREBY DISCLAIMS ANY AND ALL WARRANTIES FOR SUCH USE. Nothing in this document should be construed as altering, waiving or amending in any manner 10x Genomics terms and conditions of sale for the Chromium Controller or the Chromium Single Cell Controller, consumables or software, including without limitation such terms and conditions relating to certain use restrictions, limited license, warranty and limitation of liability, and nothing in this document shall be deemed to be Documentation, as that term is set forth in such terms and conditions of sale. Nothing in this document shall be construed as any representation by 10x Genomics that it currently or will at any time in the future offer or in any way support any application set forth herein.

Contact:Email: support@10xgenomics.com

10x Genomics

6230 Stoneridge Mall Road

Pleasanton, CA